



Competence in Labware

Labware range



Welcome!

VITLAB has over 100 years of tradition. The company VITRI GmbH & Co. KG was established in 1908 in Mühlthal, and the laboratory division was spun off in 1989 as VITLAB. Today, VITLAB is one of the leading manufacturers of liquid handling instruments and performance plastic laboratory products for one-time or long-term use. We develop and manufacture these laboratory products at our own production facility.

Our extensive range of products provides optimal support in your laboratory work in a wide variety of application ranges. Regardless of whether your work involves volume measurement, sampling or storage: VITLAB products will facilitate it while continuing to ensure that you achieve perfect results.

We hope that this new catalogue will serve as a valuable resource to aid in your lab work. We would be glad to respond to your enquiries, and look forward to receiving suggestions and ideas from our users.



This catalogue describes our products and provides all essential information. You will find detailed data regarding the various plastics clearly presented in the chapter entitled “General and Technical Information”. To simplify your search, our product range has been categorised into the following areas of application: dispensing, pipetting, titration, volume measurement, measuring and transferring, sample preparation, saving and storing, lab assistants.

Under “Volume Measurement”, for example, you will find a wide variety of classical volumetric instruments such as volumetric flasks, measuring cylinders, and associated accessories.

In addition to the range of products that appears in our catalogue, we also produce plastic products according to customer specification. For example, bottles and beakers required for special tasks can be commissioned with a specified geometry and thickness. Optionally, the products can be printed with an individualised scale or with customised labelling. Labware for promotional use can be designed and printed with a company name and logo. We can even accommodate requests for individualised packaging formats, materials, and designs. Further information is available in the VITLAB® Promotional chapter.

Many possibilities can be realised – don’t hesitate to ask what we can do for you!





VITLAB

Your reliable p



Certified quality

Independent inspections and routine internal audits guarantee the effectiveness of VITLAB's quality management system throughout the entire company, from development to shipment. As a result, the phrase 'Made by VITLAB' has become synonymous with quality.



Over 98% of our product line is made in Germany. Supplemental procedures such as tempering and volume testing are conducted in our own facilities, which guarantees the highest possible product quality and measurement accuracy. Our continuous improvement paradigm supports our goal of 0% failure.



The VITLAB Quality Management System has been continuously certified since January 1994, according to DIN EN ISO 9001. Active stewardship of the environment is an equally strong pillar of our business philosophy. VITLAB has been certified according to DIN EN ISO 14001 since May, 1999.

artner



Prompt deliveries Competent customer service


The highly efficient logistics in the Großostheim production facility facilitate the shortest possible delivery times for all products listed in the catalogue. For the standard articles, we strive for an availability of over 94%.

Due to its intensive partnerships with distributors in over 70 countries, VITLAB can offer sound on-site advice, individual support, and quick answers to your questions. Our qualified product training sessions provide comprehensive technical and application-oriented information on using our products. Should problems arise, our expert repair service keeps downtime as short as possible.

VITLAB products can be ordered from specialist dealers worldwide. Our authorised sales partners can be found on the internet at:

www.vitlab.com

Or contact us directly.

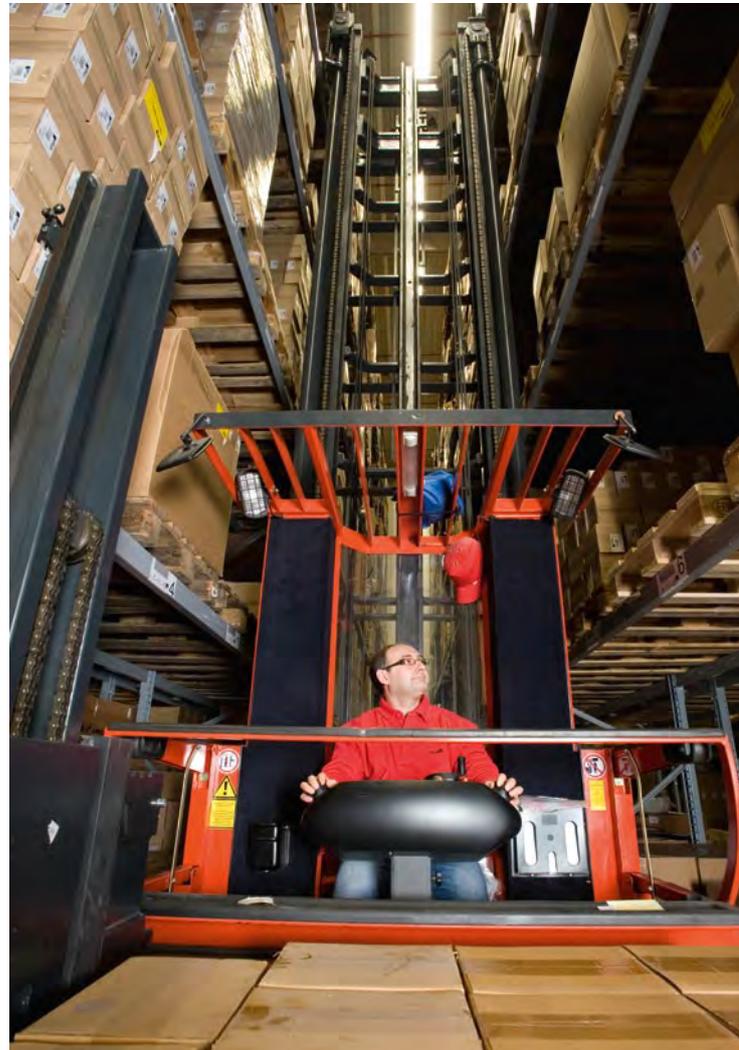

For your information



Your contact Customer Service

Our Customer Service staff is at your service to provide you with competent advice and answers to all your queries and questions concerning offers, orders and deliveries. Our Product Management and Sales Team are at your disposal – also “on site” – with any technical information or assistance that you might require for your application.

VITLAB GmbH, Customer Service

tel: +49 (0) 6026 9 77 99-0
fax: +49 (0) 6026 9 77 99-30
e-mail: info@vitlab.com
web: www.vitlab.com

Please understand that technical specifications, catalogue numbers and designs may change after this catalogue is published. The illustrations used are for representation only, and the details may vary from the description. All measurements, with the exception of exact tolerances, should be understood as approximate values. Please keep in mind that the actual testing and measuring results can be influenced by a variety of factors that are beyond our control. Therefore, you should carefully check the transferability of the data applying it to a particular application.

The packaging units (PU) correspond to the minimum order quantities. All up-to-date information is also available on the internet at www.vitlab.com.

If you need additional information, please call us.

VITLAB  , **VITLAB** [®] ,
maneus [®] , **pipeo** [®] , **VITsafe** [™]
are brands of **VITLAB GmbH**.

Table of contents

Dosing

Bottle-top dispensers and accessories

Starting on page 9



Pipetting

Micropipettes, tips and accessories

Starting on page 21



Titration

Bottle-top burettes, burettes and accessories

Starting on page 29



Volume measurement

Volumetric flasks, graduated cylinders, pipettes, pipette helpers and accessories

Starting on page 35



Measuring and transferring

Graduated beakers, scoops, spatula, forceps, funnels and accessories

Starting on page 55



Sample preparation

Wash bottles, dropping bottles, dropping pipettes, spray bottles, Griffin beakers, watch glasses, Erlenmeyer flasks, magnetic stirring bars, mortars, pestles, equipment for material separation, desiccators, sample vials, staining cuvettes and accessories

Starting on page 65



Saving and storing

Lab bottles, reagent bottles, storing bottles and transport containers

Starting on page 103



Lab assistants

Connectors, valves, trays, drawer organisers and drying racks

Starting on page 117



VITLAB® Promotional

Starting on page 125



General and technical information

Starting on page 129



Clear product statements

Our aim is to provide you with a clear and comprehensive presentation of all relevant product information. For quick reference, we use the following symbols:



DIN ISO-compliant Class A volumetric instruments



DE-M marking for conformity certified products according to the German Measurement and Calibration Regulation



Food-safe products according to EU Directive No. 10/2011



Products with high protection for light-sensitive substances



Products individually packaged in PE bags, labelled with the article number, description and EAN code



Products that can be autoclaved at 121 °C (2 bar) according to DIN EN 285. Note restrictions!



CE mark according to EU Guideline 2004/108/EC, 93/68/EEC; 73/23/EEC, and 93/68/EEC



CE-IVD mark according to EU Guideline 98/79/EC

Perfection in Liquid Handling

HIGHEST RELIABILITY IN DISPENSING



VITLAB 
Competence in Labware

VITLAB® Dispenser line: genius, simplex, and TA

VITLAB bottle-top dispensers are available for a broad spectrum of applications in the dispensing of exact volumes. VITLAB® genius and simplex can be used for practically any task, while VITLAB® TA dispensers have been specially developed for use in trace analysis and with highly concentrated media. As they are produced from materials with extremely high chemical resistance, VITLAB® bottle-top dispensers are very robust and reliable.



	VITLAB® genius/simplex	VITLAB® TA
Applications	Salt solutions, acids, bases, and many organic solvents	Specially for use in trace analysis for dispensing high-purity and highly concentrated acids and alkalis, as well as hydrogen peroxide, bromine and HF
Components in contact with media	Borosilicate glass, FEP, ETFE, PFA, PTFE, platinum-iridium, PVDF (screw cap)	Various fluoroplastics (e.g., ETFE, FEP, PFA, PTFE), Al ₂ O ₃ -sapphire, platinum-iridium or tantalum (depending on the model)
Operating limits	Temperature: +15 °C to +40 °C Steam pressure: max. 500 mbar Viscosity: max. 500 mm ² /s Density: max. 2.2 g/cm ³	Temperature: +15 °C to +40 °C Steam pressure: max. 600 mbar Viscosity: max. 500 mm ² /s Density: max. 3.8 g/cm ³

* Dynamic viscosity [mPas] = kinematic viscosity [mm²/s] x density [g/cm³]

General guide for dispenser selection (for the classification of dispenser media, see page 11).

Salt solutions	Acids and bases	Solvents	High-purity and highly concentrated acids and bases	Hydrofluoric acid (HF), bromine, hydrogen peroxide
VITLAB® genius/simplex →		VITLAB® genius/simplex →		
			VITLAB® TA →	

Dosing

Recommended usage ranges for VITLAB® genius and VITLAB® simplex:

Medium	Medium	Medium
O Acetaldehyde	O Chloronaphthalene	I Hydrochloric acid, 37%
O Acetone	I Chromic acid	O Lactic acid
O Acetonitrile	I Chromic-sulphuric acid	I Magnesium chloride
O Acetylacetone	I Copper sulphate	I Mercury chloride
O Acrylic acid	O Cresol	O Methanol
O Acrylonitrile	O Cumene (isopropylbenzene)	O Methoxybenzene
O Adipic acid	O Cyclohexanone	O Methyl butyl ether
O Allyl alcohol	O Decane	O Methyl formate
I Aluminium chloride	O 1-Decanol	O Methyl propyl ketone
O Amino acids	O Di(ethylene glycol)	O Mineral oil (motor oil)
I Ammonium chloride	O Dibenzyl ether	O Monochloroacetic acid, 50%
I Ammonium fluoride	O Dichlorobenzene	I Nitric acid, 60%
I Ammonium hydroxide	O Dichloroethane	O Nitrobenzene
I Ammonium sulphate	O Dichloromethane	O Octane
O Amyl acetate	O Diethanolamine	O Oleic acid
O Amyl alcohol (pentanol)	O Diethyl ether	O Oxalic acid
O Amyl chloride (chloropentane)	O Diethylamine	I Perchloric acid
O Aniline	O 1,2 Diethylbenzene	O Petroleum
I Barium chloride	O Dimethyl sulphoxide (DMSO)	O Phenol
O Benzaldehyde	O Dimethylaniline	O Phenylethanol
O Benzene	O Dimethylformamide (DMF)	O Phenylhydrazine
O Benzoyl chloride	O 1,4 Dioxane	I Phosphoric acid, 85%
O Benzyl alcohol	O Diphenyl ether	I Phosphoric acid, 85% + sulphuric acid, 98%, 1:1
O Benzyl chloride	O Ethanol	O Piperidine
O Benzylamine	O Ethanolamine	O Propanol
I Boric acid	O Ethyl acetate	O Propionic acid
O Bromobenzene	O Formaldehyde	O Propylene glycol (propanediol)
O Bromonaphthalene	O Formamide	O Propylene oxide
O Butanediol	O Glacial acetic acid	O Pyridine
O 1-Butanol	O Glycerine	O Salicylaldehyde
O n-Butyl acetate	O Glycol (ethylene glycol)	O Salicylic acid
O Butyl methyl ether	O Glycolic acid, 50%	O Silver acetate
O Butylamine	O Heating oil (Diesel oil)	I Silver nitrate
O Butyric acid	O Hexane	O Sodium acetate
I Calcium carbonate	O Hexanoic acid	I Sodium chloride
I Calcium chloride	O Hexanol	I Sodium dichromate
I Calcium hydroxide	I Hydroiodic acid	I Sodium fluoride
I Calcium hypochlorite	I Iodine / potassium iodide solution	I Sodium hydroxide, 30%
O Chloroacetaldehyde	O Isoamyl alcohol	I Sodium hypochlorite
O Chloroacetic acid	O Isobutanol	I Sulphuric acid, 98%
O Chloroacetone	O Isopropanol (2-propanol)	O Tartaric acid
O Chlorobenzene	O Isopropyl ether	O Tetramethylammonium hydroxide
O Chlorobutane	O Methyl ethyl ketone	O Toluene
O Formic acid	I Potassium chloride	O Turpentine
O Gasoline	I Potassium dichromate	O Xylene
O Methyl benzoate	I Potassium hydroxide	I Zinc chloride
O Pyruvic acid	I Potassium permanganate	I Zinc sulphate
O Acetic acid	O Urea	

The above data have been carefully checked and reflect the current state of knowledge. Always follow the instructions for use that accompany the instrument as well as the reagent manufacturer's instruction manual. In addition to the chemicals listed above, solutions of a wide variety of organic or inorganic salts (e.g., biological buffers), biological detergents, and cell culture media can be dispensed. Should you require information on chemicals not listed, please do not hesitate to contact us. Last updated: 03/12.

I Inorganic media

O Organic media

VITLAB® genius & simplex



Drawing quantities of liquids from large supply bottles is a daily routine in the lab. This manual task must be carried out quickly, accurately, reproducibly, simply and safely.

VITLAB® genius and simplex bottle-top dispensers are a family of instruments with proven precision that offer many advantages in routine liquid-handling operations. VITLAB® genius and simplex can be used in practically any operation and are suitable for **organic and inorganic solutions**. The materials that come in contact with media (PTFE, PFA, FEP, borosilicate glass and platinum-iridium) are resistant to most acids, bases, and solvents.

VITLAB® genius and simplex are equipped with a positive displacement piston and a fluoroplastic (PFA) sealing lip on the cylinder wall. The latter acts like a windscreen wiper **to prevent crystal build-up on the cylinder wall** from readily crystallisable media. The glass cylinder is also coated with a plastic material that reduces the risk of splashes should breakage occur. The telescopic filling tube can be adjusted smoothly to different bottle heights.

VITLAB® genius is also equipped with our patented recirculation valve (EP 542 241) that reduces reagent loss when ventilated. The simple-to-use calibration function of the VITLAB® genius helps to meet all of the requirements of testing-apparatus monitoring, with the minimum of downtime.

VITLAB® genius and simplex are completely autoclavable at 121 °C (2 bar) according to DIN EN 285, and are DE-M marked. Also available with DAkkS calibration certificate or individual quality certificate.

Included in delivery:

VITLAB® genius or VITLAB® simplex with 3 threaded adapters made from PP.
Nominal volumes of 2.5 - 10 ml (screw coupling GL 32) with adapters GL 28, S 40 and GL 45.
Nominal volumes of 25 - 100 ml (screw coupling GL 45) with adapters GL 32, GL 38 and S 40.
Telescopic filling tube (200 - 350 mm), mounting tool, instruction manual, and quality certificate stating all test values.

Volume ml	Graduation ml	A* ≤ ± %	CV* ≤ %	PU	VITLAB® simplex Cat. No.	VITLAB® genius Cat. No.
--------------	------------------	-------------	------------	----	--------------------------------	-------------------------------

VITLAB® simplex/genius

0.25 - 2.5	0.05	0.6	0.1	1	1601503	1605503
0.5 - 5.0	0.10	0.5	0.1	1	1601504	1605504
1.0 - 10.0	0.20	0.5	0.1	1	1601505	1605505
2.5 - 25.0	0.50	0.5	0.1	1	1601506	1605506
5.0 - 50.0	1.00	0.5	0.1	1	1601507	1605507
10.0 - 100.0	2.00	0.5	0.1	1	1601508	1605508

VITLAB® simplex fix

1.0	-	0.6	0.1	1	1602502	
5.0	-	0.5	0.1	1	1602504	
10.0	-	0.5	0.1	1	1602505	

* Error limits according to DIN EN ISO 8655-5. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. DE-M marked.



Dosing

Bottles for VITLAB® genius and simplex

Reagent bottles made of Polypropylene. Transparent.
 With screw cap made of PP.
 Good chemical resistance, ideal for long-term storage of liquids.
 Autoclavable at 121 °C (2 bar) according to DIN EN 285.
 Food-safe products according to EU Directive No. 10/2011.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
500	25	165	87	10	100589
500	45	172	87	10	101789
1000	32	202	108	10	100689
1000	45	197	105	10	102089
2000	32	245	131	6	100789
2000	45	241	131	6	102189



Threaded brown glass (soda lime glass) bottles with an ethylene acrylate coating for increased safety, and a screw cap. The plastic coating significantly reduces hazardous glass splintering during breakage. The maximum working temperature for coated bottles is 80 °C. To preserve the coating, do not clean at temperatures exceeding 60 °C.

Volume	Form	Bottle neck threads GL	PU	Cat. No.
100	round	GL 28	1	1671505
100	square	GL 32	1	1671506
250	square	GL 32	1	1671515
500	square	GL 32	1	1671520
1000	square	GL 45	1	1671500
2500	round	GL 45	1	1671510



Plastic stand for VITLAB® dispensers

For secure anchoring, made entirely of polypropylene for contamination-free operation (no metal). Suitable for VITLAB® dispensers with screw coupling GL 45.
 Stand rod: 325 mm; base: 220 x 160 mm; weight: 1,130 g.

Description	PU	Cat. No.
Plastic stand	1	1671116





Drying tube for VITLAB® genius and simplex

PP, transparent, unfilled. Can be connected directly to the dispenser.

Description	PU	Cat. No.
Drying tube, PP, unfilled	1	1671095



Discharge tube for VITLAB® genius and simplex

Including collection tube with joist, dosing needle with flexible discharge tube (80 cm, PTFE) and handle and assembly instructions.

Description	PU	Cat. No.
Discharge tube for simplex / genius 2.5, 5 and 10 ml	1	1650086
Discharge tube for simplex / genius 25, 50 and 100 ml	1	1650111



Adapter for VITLAB® genius and simplex

Made of PP, for screwing the dispensers onto the reagent bottles with an NS neck, GL screw thread or an S buttress thread.

Description	External thread	Bottle neck threads	PU	Cat. No.
NS-adapter	GL 32	NS 19/26	1	1670066
NS-adapter	GL 32	NS 24/29	1	1670067
NS-adapter	GL 32	NS 29/32	1	1670068
Thread adapter	GL 32	GL 25	1	1670150
Thread adapter	GL 32	GL 28	1	1670155
Thread adapter	GL 32	GL 38	1	1670165
Thread adapter	GL 32	GL 45	1	1670175
Thread adapter	GL 32	S 40	1	1670170
Thread adapter	GL 45	GL 32	1	1670180
Thread adapter	GL 45	GL 38	1	1670110
Thread adapter	GL 45	S 40	1	1670120

Adapters made of ETFE/PTFE can be found on page 31.

Dosing

Filling tubes for VITLAB® genius and simplex

Description	Length mm	PU	Cat. No.
Telescopic filling tube, FEP, ETFE, PTFE, for all sizes	200 - 350	1	1671085
Filling tube, FEP, for simplex/genius 2.5, 5 and 10 ml	220	1	1650020
Filling tube, FEP, for simplex/genius 2.5, 5 and 10 ml	335	1	1650025
Filling tube, FEP, for simplex/genius 25, 50 and 100 ml	250	1	1650030
Filling tube, FEP, for simplex/genius 25, 50 and 100 ml	335	1	1650035



Discharge tube for VITLAB® genius and simplex

Discharge tube made of FEP.

Including discharge tube securing nut (PP) and discharge tube closing cap (PVDF).

Size ml	PU	VITLAB® simplex Cat. No.	VITLAB® genius Cat. No.
2.5 / 5 / 10	1	1650080	1650085
25 / 50 / 100	1	1650100	1650110





Discharge valve for VITLAB® genius

Combined discharge and recirculation valve for dispenser VITLAB® genius made of PTFE, PFA, borosilicate glass 3.3 and platinum-iridium.

Size ml	PU	Cat. No.
2.5 / 5 / 10	1	1655075
25 / 50 / 100	1	1655080



Discharge valve for VITLAB® simplex

Discharge valve for VITLAB® simplex made of PFA, borosilicate glass 3.3 and platinum-iridium.

Size ml	PU	Cat. No.
2.5 / 5 / 10	1	1655095
25 / 50 / 100	1	1655100

Dosing

VITLAB® TA



The VITLAB® TA dispenser is the dosing device of choice to meet the demanding purity standards required in trace analysis. The high quality parts that come exclusively in contact with the medium and the specially developed and proven cleaning process to be done before use results in **a reduced release of trace metal ions to the low ppb range, or, depending on the application, even the ppt range**. The parts that are in contact with media are made of various fluoroplastics (e.g. ETFE, FEP, PFA, PTFE), Al₂O₃-sapphire, platinum-iridium or tantalum (depending on model).

Thanks to the excellent chemical resistance of the materials used, the new dispenser can also be deployed with **highly concentrated acids and bases**, such as perchloric, sulphuric and nitric acid. Depending on the application, there is a choice of two different valve spring systems: the VITLAB® TA with tantalum spring is recommended for dosing of hydrogen peroxide (H₂O₂). For applications using sodium hydroxide (up to a max. concentration of 30%) or hydrogen fluoride (HF) the platinum-iridium spring is recommended. In order to minimize the loss of valuable reagents or sample solutions, VITLAB offers the dispenser with the optional recirculation valve. Also available with DAKkS calibration certificate or individual quality certificate.

Included in delivery:

VITLAB® TA dispenser (screw thread GL 45) with adjustable variable volumes, DE-M marked, with quality certificate, telescopic filling tube, mounting tool, GL 28/S 28 (ETFE), GL 32 (ETFE), and S 40 (PTFE) bottle adapters, and instruction manual. Optionally with or without recirculation valve.

Volume ml	Valve spring	Recirculation	Graduation ml	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
1.0 - 10.0	Pt-Ir	no	0.2	0.5	0.1	1	1607515
1.0 - 10.0	Pt-Ir	yes	0.2	0.5	0.1	1	1607525
1.0 - 10.0	Ta	no	0.2	0.5	0.1	1	1607535
1.0 - 10.0	Ta	yes	0.2	0.5	0.1	1	1607545

* Error limits according to DIN EN ISO 8655-5. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. DE-M marked.



Recommended dispensing media for VITLAB® TA

Dispensing medium	Valve spring: Pt-Ir	Valve spring: Ta
Acetic acid	+	+
Ammonia solution	+	+
Bromine	+	+
Hydrochloric acid	+	+
Hydrofluoric acid*)	+	-
Hydrogen peroxide	-	+
Nitric acid	+	+
Perchloric acid	+	+
Phosphoric acid	+	+
Sodium hydroxide, 30%	+	-
Sulphuric acid	+	+
Water	+	+

+ suitable / - unsuitable

*) Note: Hydrofluoric acid reacts slightly with sapphire resulting in slightly increased aluminium levels. To reduce these values we recommend discarding 3-5 dosings of 2 ml each before performing analysis.



Wide-mouth bottles, PFA



Transparent.

With screw cap made of PFA with buttress threads. Ideal for long-term storage of high-purity oxidants, acids, alkalis, as well as hydrocarbons, trace analysis solvents and standards.

Volume ml	Thread	Height mm	Ø mm	PU	Cat. No.
500	S 40	179	76	1	109597
1000	S 40	217	96	1	109697
2000	S 40	245	130	1	109797



Recirculation valve for VITLAB® TA

Exchangeable, choice between tantalum and platinum-iridium depending on the application.

Valve spring	PU	Cat. No.
Platinum-iridium	1	1671050
Tantalum	1	1671055



Dispensing cartridge for VITLAB® TA

Calibrated, including safety ring, with quality certificate. Nominal volume 10 ml.

Description	PU	Cat. No.
Dispensing cartridge	1	1670700



Plastic stand for VITLAB® TA

For secure anchoring, made entirely of polypropylene for contamination-free operation (no metal). Stand rod: 325 mm; base: 220 x 160 mm; weight: 1,130 g.

Description	PU	Cat. No.
Plastic stand	1	1671116

Dosing

Telescoping filling tube for VITLAB® TA

Individually adjustable lengths.

Description	Length mm	PU	Cat. No.
Telescopic filling tube, FEP, PTFE	70 – 140	1	1671080
Telescopic filling tube, FEP, PTFE	125 – 240	1	1671082
Telescopic filling tube, FEP, PTFE	195 – 350	1	1671083
Telescopic filling tube, FEP, PTFE	250 – 480	1	1671086



Adapter for VITLAB® TA

For screwing the dispenser onto reagent bottles with GL screw thread or an S buttress thread.

Description	External thread	Bottle neck threads	PU	Cat. No.
Thread adapter, ETFE	GL 32	GL 25	1	1670072
Thread adapter, ETFE	GL 32	GL 28	1	1670080
Thread adapter, ETFE	GL 32	GL 38	1	1670090
Thread adapter, ETFE	GL 32	GL 45	1	1670105
Thread adapter, ETFE	GL 32	S 40	1	1670092
Thread adapter, ETFE	GL 45	GL 32	1	1670100
Thread adapter, ETFE	GL 45	GL 38	1	1670115
Thread adapter, PTFE	GL 45	S 40	1	1670125





VITLAB® piccolo

For dispensing tiny quantities of liquids in all areas of biochemical and medical research.

Even the **smallest quantities can be dispensed directly from the bottle** with the VITLAB® piccolo - a big help, particularly for serial dispensing operations. Special advantage: Disposable tips are unnecessary. This reduces costs.

The ergonomic design makes dispensing effortless and stress-free. The VITLAB® piccolo **can be operated with only one hand**. Use the thumb to depress the volume dispensing button, just as with a pipette, and a reset mechanism refills the volume automatically.

The discharge tube can be rotated over 360° so that it is always optimally situated with respect to the bottle label.

The VITLAB® bottletop dispensers piccolo 1 and piccolo 2 are used mainly in connection with aqueous and highly diluted agents. Only high-quality materials, such as PTFE, PFA, ETFE, FEP, borosilicate glass, and platinum-iridium come in contact with the media.

VITLAB® piccolo 1 with a fixed volume

VITLAB® piccolo 2 with two fixed volumes

Also available with DAkkS calibration certificate or individual quality certificate.

Included in delivery:

VITLAB® piccolo 1 or 2 with GL 28 connecting threads, mounting tool, and instruction manual.

Type	Volume µl	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
piccolo 1	100	3.0	0.4	1	1610501
piccolo 1	200	2.5	0.4	1	1610502
piccolo 1	250	2.0	0.4	1	1610503
piccolo 1	500	1.5	0.3	1	1610504
piccolo 1	1000	1.0	0.2	1	1610506
piccolo 2	100 / 250	2.0	0.4	1	1611503
piccolo 2	500 / 1000	1.0	0.2	1	1611506
piccolo 2	1000 / 2000	1.0	0.2	1	1611508

* Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation.

Other volumes available upon request.



Adapter for VITLAB® piccolo

For screwing the dispenser onto reagent bottles with GL screw thread.

Description	External thread	Bottle neck threads	PU	Cat. No.
Thread adapter, PP, piccolo	GL 28	GL 32	1	1670145

Perfection in Liquid Handling

PRECISE AND CONVENIENT PIPETTING



VITLAB [®]
Competence in Labware

VITLAB® micropipette



The VITLAB® piston-operated pipettes are the ideal manual pipettes for demanding laboratory applications, and have all the features required by users: robust, with ergonomic shape and simple operation, completely autoclavable, highly accurate with simple calibration for long-lasting reliability.

The large, central pipetting button provides a uniform and smooth movement of the piston. For rapid replacement of the tips, the ergonomic eject button is placed easily accessible to the thumb on the front side. The VITLAB® micropipette is easy to use for both right- and left-handers. The 4-digit volume display with integrated zoom function and vertical arrangement of the numbers (top to bottom reading direction) ensures an **optimal readability of the volume** at all times. The desired volume can be set by rotating the volume-setting wheel with ease and precision. The clearly visible colour-coded frame of the volume display allows easy selection of the right pipette tip.

If necessary, e.g. for applications with non-aqueous solutions, the **integrated calibration function allows an adjustment without tools directly in the laboratory**. The corrosion-resistant piston and ejector ensure a long product life.

The micropipette is DE-M marked, CE-IVD compliant and is completely autoclavable at 121 °C (2 bar) according to DIN EN 285. Also available with DAkKS calibration certificate or individual quality certificate.

Included in delivery: VITLAB® micropipette, silicone oil resp. grease (size 5 and 10 ml), sample bag with pipette tips, quality certificate, and instruction manual.

Volume µl	A* ≤ ± %	CV* ≤ %	Tip µl	PU	Cat. No.
0.5 - 10	1.0	0.5	20	1	1641000
2 - 20	0.8	0.4	200	1	1641002
10 - 100	0.6	0.2	200/300	1	1641004
20 - 200	0.6	0.2	200/300	1	1641006
100 - 1000	0.6	0.2	1000	1	1641008
500 - 5000	0.6	0.2	5000	1	1641010
1000 - 10000	0.6	0.2	10000	1	1641012

* Calibrated to deliver 'Ex'. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. The error limits are under those specified in DIN EN ISO 8655-2. DE-M marked.

Pipetting

VITLAB® micropipette -8/-12



The VITLAB® micropipettes -8 and -12 are characterized by their especially user-friendly operation while pipetting long series. They have all the features required by users: robust, completely autoclavable and highly accurate, with simple calibration for long lasting reliability, especially for established multichannel pipette applications, such as immunological assays, dilution series, or use with cell cultures in microtiter plates.

By using innovative plastic materials, the VITLAB® multichannel pipettes are **at the same time very robust and light-weight**. To ensure a long operating life, the plastic materials used are corrosion-resistant. The ergonomic finger rest coupled with the low weight contribute to comfortable handling of the pipettes. To provide an optimal and comfortable working position, the manifold can be rotated freely 360° in both directions.

The large, central pipetting button provides uniform and smooth movement of the piston. In addition, the short stroke of 12.5 mm reduces the risk of muscular disorders as a consequence of repeated stress, such as "Repetitive Strain Injury Syndrom" (RSI). The combination of the stepped design of the ejector and special rings made of FKM reduce the effort needed for ejecting the tips and thus provide comfortable operation of the pipette.

The multichannel pipettes are **especially service-friendly** for care and maintenance, as well as for calibration. If necessary, e.g. for applications with non-aqueous solutions, the integrated calibration function allows an adjustment without tools directly in the laboratory. Single shafts and seals can be easily removed, and thus can be directly cleaned or replaced.

The VITLAB® micropipette -8 and -12 are DE-M marked, CE-IVD compliant, and are completely autoclavable at 121 °C (2 bar) according to DIN EN 285. Also available with DAkkS calibration certificate or individual quality certificate.

Included in delivery: VITLAB® micropipette -8 or -12, mounting tool for nose cones, silicone grease, 8 or 12 V-rings including instructions and mounting plus demounting tool, quality certificate and instruction manual.

Volume µl	A* ≤ ± %	CV* ≤ %	Tip µl	PU	Cat. No.
micropipette -8					
0.5 - 10	1.6	1.0	20	1	1608000
5 - 50	0.8	0.4	200	1	1608002
10 - 100	0.8	0.3	200/300	1	1608004
20 - 200	0.8	0.3	200/300	1	1608006
30 - 300	0.6	0.3	300	1	1608008
micropipette -12					
0.5 - 10	1.6	1.0	20	1	1612000
5 - 50	0.8	0.4	200	1	1612002
10 - 100	0.8	0.3	200/300	1	1612004
20 - 200	0.8	0.3	200/300	1	1612006
30 - 300	0.6	0.3	300	1	1612008

* Calibrated to deliver 'Ex'. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. The error limits are under those specified in DIN EN ISO 8655-2.

DE-M marked.



VITLAB® micropipette Starter-Sets

Each VITLAB® Starter Set includes 3 variable VITLAB® micropipettes with different volumes and associated, color-coded tip boxes, as well as 3 rack mounts for appropriate storage of your new VITLAB® micropipettes.

Our micropipettes are DE-M marked, CE-IVD compliant and are completely autoclavable at 121 °C (2 bar) according to DIN EN 285.



Starter Set "Mini"

Scope of delivery:

- VITLAB® micropipette 0.5 - 10 µl
- VITLAB® micropipette 10 - 100 µl
- VITLAB® micropipette 100 - 1000 µl
- Tip-Box 0.5 - 20 µl
- Tip-Box 2 - 200 µl
- Tip-Box 50 - 1000 µl
- Rack mount (3x)
- Product & application brochure

Cat. No.: 33331

Starter Set "Classic"

Scope of delivery:

- VITLAB® micropipette 2 - 20 µl
- VITLAB® micropipette 20 - 200 µl
- VITLAB® micropipette 100 - 1000 µl
- Tip-Box 2 - 200 µl (2x)
- Tip-Box 50 - 1000 µl
- Rack mount (3x)
- Product & application brochure

Cat. No.: 33332

Starter Set "Maxi"

Scope of delivery:

- VITLAB® micropipette 100 - 1000 µl
- VITLAB® micropipette 500 - 5000 µl
- VITLAB® micropipette 1000 - 10000 µl
- Tip-Box 50 - 1000 µl
- Tip-Box 0.5 - 5 ml
- Tip-Box 1 - 10 ml
- Rack mount (3x)
- Product & application brochure

Cat. No.: 33333

Pipetting

Accessories for VITLAB® micropipettes

With the practical rack mount and freely rotatable bench-top stand, VITLAB® micropipettes can be stored safely and ready to use.

Description	PU	Cat. No.
Wall mount for 1 pipette	1	1672000
Bench-top stand for 6 singlechannel or 6 multichannel instruments	1	1672002
Filter for pipette, 5 ml	25	1672010
Filter for pipette, 10 ml	25	1672012
Silicone oil for pipettes, up to 1000 µl	1	1672015
Silicone grease for pipettes 5 ml / 10 ml and multichannel pipettes	1	1672016
Fluorostatic grease for multichannel pipettes	1	1670050



Reagent reservoir, non-sterile, PP



Transparent, with lid to guard against contamination and spilling out of contents during movement. Optimally suited for working with multichannel pipettes. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	PU	Cat. No.
60	10	319099



Pipette tip selection guide

Which pipette tip will fit my VITLAB® micropipette?

Nominal volume VITLAB® micropipettes							Nominal volume VITLAB® micropipette -8/-12				Tip volume
10 µl	20 µl	100 µl	200 µl	1000 µl	5 ml	10 ml	50 µl	100 µl	200 µl	300 µl	
◆											0.5 - 20 µl
	◆	◆	◆				◆	◆	◆		2 - 200 µl
		◆	◆				◆	◆	◆	◆	5 - 300 µl
				◆							50 - 1000 µl
					◆						0.5 - 5 ml
						◆					1 - 10 ml



High purity

Applications in molecular biology and biochemical analysis require a high level of purity in order not to adulterate results of experiments. Molecules and enzymes such as DNA, RNases and endotoxins are very stable and cannot be completely inactivated or destroyed by sterilization procedures. RNases may even fold back after denaturation. When working with microorganisms and nucleic acids a common difficulty is their ubiquitous occurrence (on hands, in saliva); therefore, for example, it is essential to wear gloves. To avoid contamination with nucleic acids, proteins and microorganisms from human contact,

the production process of our pipette tips is largely automated in a cleanroom.

ATP is a good indicator for the presence or absence of biological contamination. It is a high-energy molecule that is produced by all living cells. Because of their ability to cut DNA or RNA, contamination with DNA, DNases and RNases can, for example, manipulate biomolecular amplification techniques such as PCR. To prevent enzymatic degradation, it is of major importance, that pipette tips are free of RNases.

Packaging variations

VITLAB® pipette tips remain available in the variations palletized in the Tip-Box and packed in bags. Additionally, empty Tip-Boxes for self-filling are available. Due to the new design and functionality, Tip-Boxes up to 1000 µl are stackable and their format now conforms to the common 96 (8x12) unit format.



NEW: Resealable bags

All tips up to 1000 µl are produced under cleanroom conditions, automatically shrink-wrapped in reclosable bags and packaged in cartons. The article number, volume range and lot number of the tips are printed on every bag.



NEW: Tip-Box (up to 1000 µl)

PP box with functional hinged and snap-on lid. For all volume ranges up to 1000 µl in practical 8x12 format. Stackable and autoclavable at 121 °C according to DIN EN 285.



Tip-Box 5/10 ml

PP box with fitted lid. Filled with 5 ml (28 pcs.) or 10 ml (18 pcs.) tips. The box is autoclavable at 121 °C according to DIN EN 285.

Pipetting

VITLAB® pipette tips are made from high-quality polypropylene and are autoclavable at 121 °C (2 bar) according to DIN EN 285. The raw material used is free from additives such as DiHEMDA (di(2-hydroxyethyl) methyl dodecyl ammonium) and oleamide (9-octadecenamide) that often cause interference, particularly in biological labs. All palletized pipette tips up to 1000 µl are from now on **free of DNA (< 40 fg), RNase (< 8.6 fg), endotoxins (< 1 pg) and ATP (< 1 fg)**.

The pipette tips are **DE-M marked, CE marked according to the IVD guideline 98/79 EC** and optimally suited for VITLAB® micropipettes.

Furthermore, the tips are compatible with most pipette models from BRAND, GILSON®, Thermo Fisher Scientific FINNPIPETTE®, Eppendorf® and sartorius® Biohit®. The 5 ml tip is only tested for VITLAB, BRAND and Thermo Fisher Scientific FINNPIPETTE®. The 10 ml tip is only tested for VITLAB, BRAND, Eppendorf® and GILSON®. Note: Pipette shafts are subject to modification and should be checked before use. The fit depends on the manufacturer, pipette type, serial number, and date of manufacture, among other things.

Pipette tips, 0.5 – 20 µl



PP, non-sterile with graduation at 2 and 10 µl. Length: 46 mm. Slim tip for contact-free pipetting into microtiter plates. Tip-Box with gray mounting plate for easy identification; palletized tips are colourless.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 1000 tips	2000	148894
Bag, Maxi	10 bags with 1000 tips	10000	155494
Tip-Box, filled	Box with 96 tips on gray mounting plate	5	149794
Tip-Box, empty	Box with gray mounting plate, without tips	1	155400



Pipette tips, 2 – 200 µl



PP, non-sterile with graduation at 20 and 100 µl. Length: 50 mm. Tip-Box with yellow mounting plate for easy identification; palletized tips are colourless. Tips in bags are coloured yellow.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 1000 tips	1000	148994
Bag, Maxi	10 bags with with 1000 tips	10000	155694
Tip-Box, filled	Box with 96 tips on yellow mounting plate	5	149994
Tip-Box, empty	Box with yellow mounting plate, without tips	1	155600






Pipette tips, 5 - 300 µl



PP, non-sterile with graduation at 50, 100 and 300 µl. Length: 53 mm. Also suitable for pipettes with yellow colour-code (see selection guide p. 25). Tip-Box with green mounting plate for easy identification; palletized tips are colorless. Tips in bags are also colorless.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 1000 tips	1000	149094
Bags, Maxi	10 bags with 1000 tips	10000	155894
Tip-Box, filled	Box with 96 tips on green mounting plate	5	150094
Tip-Box, empty	Box with green mounting plate, without tips	1	155800

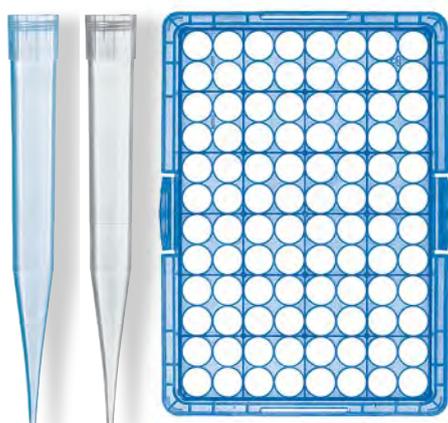

Pipette tips, 50 - 1000 µl



PP, non-sterile with graduation at 250, 500 and 1000 µl. Length: 70 mm. Tip-Box with blue mounting plate; palletized tips are colorless. Tips in bags are coloured blue.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 500 tips	1000	149194
Bags, Maxi	10 bags with 500 tips	5000	155994
Tip-Box, filled	Box with 96 tips on blue mounting plate	5	150194
Tip-Box, empty	Box with blue mounting plate, without tips	1	155900



Pipette tips, 0.5 - 5 ml



PP, non-sterile. Length: 160 mm. Diameter: approx. 9.6 mm. Slim shape for pipetting into narrow vessels such as measuring flasks with NS 12/21.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 200 tips	200	146294
Tip-Box, filled	Box with 28 tips	1	150294



Pipette tips, 1 -10 ml



PP, non-sterile. Length: 156.5 mm. Diameter: approx. 15 mm.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 100 tips	200	146494
Tip-Box, filled	Box with 18 tips	1	150394

Perfection in Liquid Handling

RAPID AND ACCURATE TITRATION



VITLAB 
Competence in Labware



VITLAB® continuous E/RS



The VITLAB® continuous bottle-top burette (Picture 1) enables continuous titration, which leads to rapid, convenient, and accurate results. The angled display shows 4-position titration volume in large, easily read numbers (Picture 2), which simplifies operation. Turning the two hand wheels supplies the titration medium in a **continuous and pulse-free** manner via the patented double-piston pump (EP 801 982) (Picture 3). Filling procedures are not necessary. This innovative technology increases safety; its compact design and low centre of gravity reduce risk of overturning, especially with smaller bottles. The height and length of the discharge tube can be adjusted, making it possible to work safely with both short and tall bottles. The patented recirculation system (EP 542 241) (Picture 4) **prevents the loss of valuable reagent** and reduces the risk of splashes. With its simple-to-use calibration function, VITLAB® continuous fulfils the corresponding requirements for test equipment monitoring without instrument downtime. Margins of error are under those specified in the DIN EN ISO 8655-3 standard, even for partial volumes. VITLAB® continuous is DE-M marked. Also available with DAKKS calibration certificate or individual quality certificate.

Included in delivery:

VITLAB® continuous E/RS, with GL 45 connecting threads and GL 32, GL 38 and S 40 (buttress thread) size PP thread adapters, telescopic filling tube (200 - 350 mm), telescopic discharge tube (140 - 220 mm), two 1.5 V microbatteries (LR 03/AAA), instruction manual, and quality certificate.

Type	Volume/rot.** ml	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
E	2.5	0.2 at 25 ml	0.1 at 25 ml	1	1620506
RS	5.0	0.2 at 50 ml	0.1 at 50 ml	1	1620507

* Error limits according to DIN EN ISO 8655-3. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. DE-M marked.

** Volume dispensed per rotation of the hand wheel

The VITLAB® continuous E/RS bottle-top burette can be used for the following titrants up to a concentration of 1 mol/L:

Acetic acid	Potassium dichromate solution
Ammonium iron (II) sulphate solution	Potassium hydroxide
Ammonium thiocyanate solution	Potassium iodate solution
Barium chloride solution	Potassium permanganate solution
Bromide bromate solution	Potassium thiocyanate solution
Cerium (IV) sulphate solution	Silver nitrate solution
EDTA solution	Sodium arsenite solution
Hydrochloric acid	Sodium carbonate solution
Iodine solution	Sodium chloride solution
Iron (II) sulphate solution	Sodium hydroxide
Nitric acid	Sodium nitrite solution
Oxalic acid solution	Sodium thiosulphate solution
Perchloric acid	Sulphuric acid
Potassium bromate solution	Tetra-n-butylammonium hydroxide solution
Potassium bromide / bromate solution	Zinc sulphate solution

The recommendations in this table have been carefully tested and reflect the most current information available. Always follow the instruction manual for the instrument as well as the reagent manufacturer's specifications. Should you require information on chemicals not listed, please do not hesitate to contact us. As at 03/12.



Titration

Adapter for VITLAB® continuous E/RS

For secure screwing of the burettes onto reagent bottles with an NS neck, GL screw thread or an S buttress thread.

Description	External thread	Bottle neck threads	PU	Cat. No.
NS-adapter, PP	GL 32	NS 19/26	1	1670066
NS-adapter, PP	GL 32	NS 24/29	1	1670067
NS-adapter, PP	GL 32	NS 29/32	1	1670068
Thread adapter, PP	GL 32	GL 28	1	1670155
Thread adapter, PP	GL 38	GL 32	1	1670085
Thread adapter, PP	GL 45	GL 32	1	1670180
Thread adapter, PP	GL 45	GL 38	1	1670110
Thread adapter, PP	GL 45	S 40	1	1670120
Thread adapter, ETFE	GL 32	GL 28	1	1670080
Thread adapter, ETFE	GL 32	GL 38	1	1670090
Thread adapter, PTFE	GL 38	GL 32	1	1670095
Thread adapter, ETFE	GL 45	GL 32	1	1670100
Thread adapter, ETFE	GL 45	GL 38	1	1670115
Thread adapter, PTFE	GL 45	S 40	1	1670125



Drying tube for VITLAB® continuous E/RS

PP, transparent, unfilled. Can be connected directly to the burette.

Description	PU	Cat. No.
Drying tube, PP, unfilled	1	1671095



Telescopic filling tube for VITLAB® continuous E/RS

For the filling of titration medium from bottles of different heights.

Description	Length mm	PU	Cat. No.
Telescopic filling tube, FEP, ETFE, PTFE	200 - 350	1	1671085



Threaded bottles for VITLAB® continuous E/RS

Threaded brown glass (soda lime glass) bottles with an ethylene acrylate coating.

Volume ml	Thread GL	Shape	PU	Cat. No.
1000	45	square	1	1671500
2500	45	round	1	1671510





VITLAB® Dr. Schilling burettes

Burettes made of borosilicate glass 3.3, tolerances according to DIN ISO 384 Class B, with high-contrast black markings. Calibrated to deliver 'Ex'. Automatic zero setting. The burette stopcock turns easily and enables fine titration. The holding device for the riser pipe serves as additional shock-proofing.

The patented VITLAB® symbiotic (DE 10 2005 034 963) offers in addition to the impact protection a thermally stable plastic coating of the glass burette tube. This provides additional breaking resistance and acts as a splinter protection.

Materials: burette of borosilicate glass 3.3, PP filling tube, PMP/PTFE burette stopcock, and PE-LD reservoir bottle.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Bottle ml	PU	Cat. No.
VITLAB® symbiotic, with Schellbach stripes (blue/white)						
25	0.05	0.05	900	1000	1	106599
50	0.10	0.10	900	1000	1	106699
Burette with Schellbach stripes (blue/white), without plastic-coating						
25	0.05	0.05	900	1000	1	106399
50	0.10	0.10	900	1000	1	106499
Burette made of brown glass, without Schellbach stripes, without plastic-coating						
25	0.05	0.05	900	1000	1	106799
50	0.10	0.10	900	1000	1	106899



Burettes, borosilicate glass 3.3

Plastic-coated burette made of borosilicate glass 3.3, tolerances corresponding to DIN ISO 384, Class B. With Schellbach stripes (blue/white) and high-contrast black marking. Calibrated to deliver 'Ex'. The burette stopcock turns easily and enables fine titration. The temperature-stable plastic coating on the tube provides splinter protection.

Materials: Burette of borosilicate glass 3.3, with PMP/PTFE burette stopcock.

Volume ml	Tolerance ± ml	Graduation ml	Length mm	PU	Cat. No.
25	0.05	0.05	800	2	105599
50	0.10	0.10	800	2	105699

Titration

Burette stopcocks, PMP/PTFE

Stopcocks made of PMP. Plugs of PTFE with polished surfaces turn easily but fit tightly. Insert with two seals.

Art. No. 105799: For tubes with an inner diameter of 7.75 ± 0.1 mm.

Art. No. 105899: For tubes with an inner diameter of 11.5 ± 0.1 mm.

For burettes ml	Height mm	Tip inner Ø mm	Installed length mm	PU	Cat. No.
25	90	1.25	17	5	105799
50	90	1.25	17	5	105899



Burette clamps, PP

Practical holder for anchoring burettes vertically on the support stand. The volume scale remains clearly readable.

Burette clamps with slip-resistant rubber-coated tips and springs made of stainless steel.

With stand clamps for securing to rods of \varnothing 8-14 mm.

Type	PU	Cat. No.
For 1 burette	5	80139
For 2 burettes	5	80140



Calibration certificates

For all volumetric instruments that are subject to test equipment monitoring, a written documentation about the regularly calibration resp. volume control is necessary. The documentation should contain the values for accuracy and coefficient of variation as well as the testing procedure and test frequency. A distinction is made between:

- Quality certificates (factory calibration report)
- Official calibration certificates (Bureau of standards, DAkkS)

Quality certificates

The VITLAB quality certificate is a factory calibration report on the basis of the quality assurance system according to DIN EN ISO 9001. Quality certificates are available as a batch or individual certificate. Devices from one production batch have the same lot number as the quality certificate. The certificate records for the specific batch the mean value, standard deviation and day of issue. In the case of an individual certificate, the volumetric instrument and the certificate bear an individual serial number in addition to the lot number. The certificate records besides the day of issue also the measured volume and the measurement uncertainty.

DAkkS calibration certificate

The DAkkS calibration certificate documents officially the traceability of measuring results to national and international standards as required by the standards DIN EN ISO 9001 and DIN EN ISO / IEC 17025 for the monitoring of measuring instruments. A major difference between factory calibration services and DAkkS laboratories is the accurate determination of the respective uncertainty of measurement guaranteed by the accredited laboratory and supervised by the DAkkS. DAkkS calibration certificates are appropriate in uses in which calibrations of an accredited laboratory are requested, where high level calibrations are demanded and for calibration of reference standards and instruments for comparative measurements.

Calibration service

VITLAB offers a repair, maintenance and calibration service (incl. DAkkS calibration) for all Liquid Handling devices made by VITLAB. The calibration laboratory accredited by the „Deutsche Akkreditierungsstelle GmbH“ (DAkkS) is authorized to issue DAkkS Calibration certificates for the following instruments: Liquid Handling products like VITLAB piston-operated pipettes and burettes, VITLAB dispensers and VITLAB volumetric plastic labware.

Competence in volume measurement

EXCELLENCE IN MEASUREMENT ACCURACY



VITLAB 
Competence in Labware



The very highest volumetric instr

Volume measurement is a routine laboratory operation. Therefore, volumetric instruments such as volumetric flasks, measuring cylinders and pipettes are standard equipment in any analytical laboratory.

The importance of the standard of measurement accuracy in your routine laboratory operations cannot be overstated. VITLAB has decades of experience in the development and production of laboratory products which are used to measure volumes. VITLAB is the first manufacturer to produce Class A measuring cylinders from PMP that are certified compliant according to DIN 12681.

All Class A PMP volumetric flasks are optionally available in transparent or UV-absorbing variations for light-sensitive substances.

High precision instruments

Calibration

Type "Ex": The delivered quantity of liquid corresponds to the volume printed on the instrument (pipettes and burettes).

Type "In": The contained quantity of liquid corresponds to the volume printed on the instrument (volumetric flasks and measuring cylinders).

VITLAB calibrates each individual volumetric flask "to contain" (In) at a reference temperature of 20 °C. The hydrophobic characteristics of the materials in plastic volumetric instruments lead to the measured volume being the same as the delivered quantity ("In" = "Ex") for aqueous solutions.

Accuracy classes

Class A: The volume tolerances lie within the limits specified by DIN and ISO.

Class B: The volume tolerances are twice the error limits for Class A specified by DIN and ISO. Detailed explanations on "accuracy in volume measurement" are available in the chapter on "General and Technical Information".

Certificate of conformity

The DE-M marking is VITLAB's guarantee that the respective products comply with the German Measurement and Calibration Regulation. The special manufacturing process developed by VITLAB, and the proven VITLAB quality management system, ensure compliance with the volume tolerances specified by the standards.





Volumetric flasks, PFA, Class A, with screw cap, PFA



Highly transparent.

Ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

The PFA screw cap guards against contamination.

Outstanding chemical resistance, can be used with strong oxidants, highly concentrated acids and alkalis, hydrocarbons, and ketones.

With laser-engraved lot number and batch certificate. Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve the ring mark, do not clean at temperatures exceeding 60 °C.

Also available with DAkkS calibration certificate or individual quality certificate.

The advantages of PFA:

- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability, suitable for volumetric instruments
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.04	90	18	1	107097
25	0.04	115	18	1	107197
50	0.06	150	18	1	107297
100	0.10	180	18	1	107397
250	0.15	235	25	1	107497
500	0.25	270	25	1	107597

* Height without screw cap

Replacement screw caps
can be found on page 105.

Compare: VITLAB® volumetric flasks ...

- ... have a circular, precisely calibrated ring mark with which the meniscus can be read accurately from any position
- ... have a straight neck for precise volume measurement
- ... have a specially formed bottom for superior stability

... are MADE IN GERMANY

Volume measurement

VITLAB® opaque volumetric flasks, PMP, Class A with NS stoppers, PP



UV-absorbing, highly transparent. For storage of light-sensitive substances.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.04	90	10/19	2	670950
25	0.04	115	10/19	2	671950
50	0.06	150	12/21	2	672950
100	0.10	180	14/23	2	673950
250	0.15	235	19/26	2	674950
500	0.25	270	19/26	2	675950
1000	0.40	310	24/29	1	676950

* Height without stopper



Replacement stoppers can be found on page 112.

VITLAB® opaque replaces brown glass and is...

- ... substantially lighter in weight
- ... practically unbreakable
- ... practically impermeable in the UV region
- ... comparable to a light protection factor of 20

VITLAB® opaque volumetric flasks, PMP, Class A, with coloured screw caps, PP



UV-absorbing, highly transparent. For storage of light-sensitive substances.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.04	90	18	2	670040
25	0.04	115	18	2	671040
50	0.06	150	18	2	672040
100	0.10	180	18	2	673040
250	0.15	235	25	2	674040
500	0.25	270	25	2	675040
1000	0.40	310	32	1	676040

* Height without screw cap



Replacement screw caps can be found on page 107.



Volumetric flasks, PMP, Class A with NS stoppers, PP



Crystal clear.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.04	90	10/19	6	67704
25	0.04	115	10/19	6	67104
50	0.06	150	12/21	6	67204
100	0.10	180	14/23	6	67304
250	0.15	235	19/26	5	67404
500	0.25	270	19/26	4	67504
1000	0.40	310	24/29	3	67604

* Height without stopper

→ Replacement stoppers
can be found on page 112. →

Volume measurement

Volumetric flasks, PMP, Class B with NS stoppers, PP



Crystal clear.

With ring mark individually calibrated to 'In'.

Class B tolerances according to DIN EN ISO 1042.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.08	90	10/19	6	67795
25	0.08	115	10/19	6	67195
50	0.12	150	12/21	6	67295
100	0.20	180	14/23	6	67395
250	0.30	235	19/26	5	67495
500	0.50	270	19/26	4	67595
1000	0.80	310	24/29	3	67695

* Height without stopper



→ Replacement stoppers can be found on page 112. →

Volumetric flasks, PMP, Class B with screw caps, PP



Crystal clear.

With ring mark individually calibrated to 'In'.

Class B tolerances according to DIN EN ISO 1042.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.08	90	18	6	677895
25	0.08	115	18	6	671895
50	0.12	150	18	6	672895
100	0.20	180	18	6	673895
250	0.30	235	25	5	674895
500	0.50	270	25	4	675895
1000	0.80	310	32	3	676895

* Height without screw cap



→ Replacement screw caps can be found on page 107. →



Volumetric flasks, PP, Class B with NS stoppers, PP



Highly transparent.
With ring mark individually calibrated to 'In'.
Class B tolerances according to DIN EN ISO 1042.
Thermal stress up to 60 °C does not permanently exceed the tolerance limits.
To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.08	90	10/19	6	677941
25	0.08	115	10/19	6	671941
50	0.12	150	12/21	6	672941
100	0.20	180	14/23	6	673941
250	0.30	235	19/26	5	674941
500	0.50	270	19/26	4	675941
1000	0.80	310	24/29	3	676941

* Height without stopper

Replacement stoppers
can be found on page 112.



Volumetric flasks, PP, Class B, with screw cap, PP



Highly transparent.
With ring mark individually calibrated to 'In'.
Class B tolerances according to DIN EN ISO 1042.
Thermal stress up to 60 °C does not permanently exceed the tolerance limits.
To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.08	90	18	6	677891
25	0.08	115	18	6	671891
50	0.12	150	18	6	672891
100	0.20	180	18	6	673891
250	0.30	235	25	5	674891
500	0.50	270	25	4	675891
1000	0.80	310	32	3	676891

* Height without screw cap

Replacement screw caps
can be found on page 107.

Volume measurement

Graduated cylinders, PMP, Class A, tall form, red printed scale



Crystal clear. DE-M marked.

With a red printed scale and ring marks at the primary scale points, calibrated 'In'.

The lot certificate supplied bears the batch number and the actual nominal value ascertained under the test conditions. The resulting deviations from the nominal value fall well under the allowed tolerances of Class A according to DIN 12681 and ISO 6706.

With printed batch number and year of production. Also available with DAkkS calibration certificate or individual quality certificate.

Hexagonal base with bottom studs provides high stability. To preserve markings, do not clean at temperatures exceeding 60 °C. Thus, conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving we recommend the design with raised graduations (Cat.-No. 64604 – 65304).

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.10	0.20	145	15	2	64614
25	0.25	0.50	170	22	2	64714
50	0.50	1.00	200	27	2	64814
100	0.50	1.00	250	33	2	64914
250	1.00	2.00	315	44	2	65014
500	2.50	5.00	360	58	1	65114
1000	5.00	10.00	440	69	1	65214
2000	10.00	20.00	535	97	1	65414



Graduated cylinders, PMP, Class A, tall shape, raised scale



Crystal clear. DE-M marked.

With a raised scale and ring marks at the primary scale points, calibrated 'In'.

The lot certificate supplied bears the batch number and the actual nominal value ascertained under the test conditions. The resulting deviations from the nominal value fall well under the allowed tolerances of Class A according to DIN 12681 and ISO 6706. With the laser engraved batch number and the year of manufacture. Also available with DAkkS calibration certificate or individual quality certificate.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 121 °C (autoclaving) does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.10	0.20	145	15	2	64604
25	0.25	0.50	170	22	2	64704
50	0.50	1.00	200	27	2	64804
100	0.50	1.00	250	33	2	64904
250	1.00	2.00	315	44	2	65004
500	2.50	5.00	360	58	1	65104
1000	5.00	10.00	440	69	1	65204
2000	10.00	20.00	482	97	1	65304





Graduated cylinders, PP, Class B, tall shape, with raised blue scale



Highly transparent.

With easily readable, raised, embossed blue scale and ring marks at the primary scale points. Calibrated 'In'. Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded. To preserve markings, do not clean at temperatures exceeding 60 °C.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.20	0.20	145	15	12	646081
25	0.50	0.50	170	22	12	647081
50	1.00	1.00	200	27	12	648081
100	1.00	1.00	250	33	12	649081
250	2.00	2.00	315	44	6	650081
500	5.00	5.00	360	58	6	651081
1000	10.00	10.00	440	69	6	652081
2000	20.00	20.00	482	97	3	653081



Graduated cylinders, PP, Class B tall shape, with a raised scale



Highly transparent.

With a raised scale and ring marks at the primary scale points, calibrated 'In'. Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.20	0.20	145	15	12	646941
25	0.50	0.50	170	22	12	647941
50	1.00	1.00	200	27	12	648941
100	1.00	1.00	250	33	12	649941
250	2.00	2.00	315	44	6	650941
500	5.00	5.00	360	58	6	651941
1000	10.00	10.00	440	69	6	652941
2000	20.00	20.00	482	97	3	653941

Volume measurement

Graduated cylinders, SAN, Class B tall shape, with a raised scale



Crystal clear.

With a raised scale and ring marks at the primary scale points, calibrated 'In'.

Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 60 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.20	0.20	140	16	12	64691
25	0.50	0.50	169	21	12	64791
50	1.00	1.00	199	28	12	64891
100	1.00	1.00	260	34	12	64991
250	2.00	2.00	315	47	6	65091
500	5.00	5.00	350	61	6	65191
1000	10.00	10.00	415	76	6	65291
2000	20.00	20.00	482	97	3	65391



Graduated cylinders, PP, Class B short shape, with a raised scale



Highly transparent.

With a raised scale, calibrated 'In'.

Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
25	0.50	0.50	122	22	12	640941
50	1.00	1.00	142	27	12	641941
100	2.00	2.00	163	37	12	642941
250	5.00	5.00	192	51	6	643941
500	10.00	10.00	218	67	6	644941
1000	20.00	20.00	285	78	6	645941





Graduated cylinders, SAN, Class B, short shape, with a raised scale



Crystal clear.

With a raised scale, calibrated 'In'.

Thermal stress up to 60 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
25	0.50	0.50	122	22	12	64091
50	1.00	1.00	142	27	12	64191
100	2.00	2.00	163	37	12	64291
250	5.00	5.00	192	51	6	64391
500	10.00	10.00	218	67	6	64491
1000	20.00	20.00	285	78	6	64591

Compare: VITLAB® graduated cylinders...

- ... have guaranteed seamless interiors, which mean the analysis is unaffected by residues and carryover
- ... have precise calibration ring marks at the primary scale points, with which the meniscus can be read accurately
- ... a sturdy, even stand for precise volume measurement

... are MADE IN GERMANY



Hydrometer cylinder, PP

Highly transparent, with spout and overflow vessel. For density measurements using a hydrometer. Hydrometer can be read through the overflow vessel with a completely filled cylinder.

With a raised scale and ring marks at the primary scale points, calibrated 'In'.

Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
500	5.00	351	73	1	760941

Volume measurement

Bulb pipettes, PP, Class B

Calibrated to deliver 'Ex'.

Highly transparent. With high-contrast, blue markings.

Break-resistant.

High chemical resistance.

Exposure to temperatures above 60 °C can lead to volume changes.

Recommended cleaning with mild alkaline detergents up to 60 °C.

Volume ml	Tolerance ± ml	Length mm	PU	Cat. No.
1	0.02	300	12	164094
2	0.02	300	12	164194
5	0.03	300	6	164294
10	0.04	440	6	164394
25	0.05	450	6	164494
50	0.10	460	6	164594



Graduated pipettes, PP, Class B

Calibrated to deliver 'Ex'.

Highly transparent. With high-contrast, blue markings.

Break-resistant.

High chemical resistance.

Outer diameter of suction tube: max. 8 mm.

Exposure to temperatures above 60 °C can lead to volume changes.

Recommended cleaning with mild alkaline detergents up to 60 °C.

Volume ml	Tolerance ± ml	Graduation ml	Length mm	PU	Cat. No.
1	0.02	0.1	300	12	163094
2	0.02	0.1	300	12	163194
5	0.05	0.1	330	12	163294
10*	0.10	0.1	330	12	163394
10	0.10	0.1	320	12	163594

* Suction tube outer diameter: 10 mm





Disposable pipettes, PS, sterile



Crystal clear, graduated, individual sterile packaging, pyrogen-free. Identified by bar-code. With cotton-wool filter.

Volume ml	Graduation ml	Length mm	PU	Cat. No.
1	0.01	272	25	160110
2	0.01	272	25	160210
5	0.10	320	25	160510
10	0.10	320	25	161010
25	0.20	345	10	162510



Disposable pipettes, PS, non-sterile

Crystal clear, graduated, non-sterile. Identified by bar-code. With cotton-wool filter.

Volume ml	Graduation ml	Length mm	PU	Cat. No.
1	0.01	272	10	160119
2	0.01	272	10	160219
5	0.10	320	10	160519
10	0.10	320	10	161019

→ Pipette helpers
can be found on pages 49 - 51. →

Volume measurement

VITLAB pipeo®



For all pipettes from 0.1 to 200 ml.

With the VITLAB pipeo® pipette controller, pipette handling is simple and comfortable. The ergonomic handle - **very light weight** at about 190 grams - and excellent balance all contribute to ease of operation. The speed can be adjusted easily, continuously and exactly with one hand using two buttons. A 50 ml pipette can be filled comfortably in less than ten seconds. The liquid release can be done either by gravity delivery when calibrated 'Ex' (to deliver), or in blow out mode using the battery-operated motor.

Pipettes are held securely and tightly in the exchangeable adapter. Liquid vapours are purged directly to protect the instrument.

One full charge of the nickel-metal hydride battery allows 8 hours of non-stop pipetting. The charge level of the recyclable battery is shown by the LED indicator. Defective batteries are easily replaced. To avoid surprises, the LED light changes from green to red two hours before the battery must be recharged. **The VITLAB pipeo® can still be operated while the battery is being recharged.**

Included in delivery:

VITLAB pipeo®, battery charger, battery, one battery compartment cover, two replacement 0.2 µm membrane filters, instruction manual.



Type	PU	Cat. No.
pipeo® with battery charger for the European continent 230 V/50 Hz	1	1631500
pipeo® with battery charger for UK/Ireland 230 V/50 Hz	1	1631510
pipeo® with battery charger for Australia 230 V/50 Hz	1	1631520
pipeo® with battery charger for Japan 100 V/50 Hz	1	1631530
pipeo® with battery charger for USA 120 V/60 Hz	1	1631540



VITLAB maneus®



The VITLAB maneus® pipette controller enables both left- and right-handers to operate all normal bulb and graduated pipettes easily and fatigue-free. Its safe and easy handling allows even inexperienced users **to adjust the meniscus precisely**.

With the new design, unscrewing the adapter enables easy and fast replacement of the hydrophobic membrane filter, which **protects the instrument against fluid penetration**.

The valve system is optimised so that liquids can be drawn up simply, without exerting pressure. The highly sensitive filling and discharge of liquids are controlled gently by the pipetting knob. Thus, the suction element provides rapid filling of the pipette (capacity: 50 ml in less than 10 seconds). The discharge bellows are used for the emptying (blow-out) of the pipette. The specially moulded intake cone ensures secure seating for all normal bulb and graduated pipettes (0.1 to 200 ml).

The VITLAB maneus® is simple to dismantle, easy to clean, and completely autoclavable at 121 °C (2 bar) according to DIN EN 285.

For all normal bulb and graduated pipettes from 0.1 to 200 ml. With replacement 3 µm membrane filter and instruction manual.

Type	PU	Cat. No.
maneus®	1	1630500



Accessories for VITLAB pipeo® & maneus®

For a detailed list of replacement parts, please see the instruction manual for the instrument, or visit our homepage: www.vitlab.com.

Description	PU	Cat. No.
Membrane filter, 0.2 µm, sterile, VITLAB pipeo®	1	1670647
Membrane filter, 0.2 µm, non-sterile, VITLAB pipeo®	10	1670648
Membrane filter, 3 µm, non-sterile, VITLAB pipeo®, VITLAB maneus®	10	1670650
Wall rack, VITLAB pipeo®	1	1670660

Volume measurement

Pipette fillers, NR

Classic accessory for pipetting with volumetric or measuring pipettes. With 3 valves.
Valve A: Air release, Valve B: Liquid filling, Valve E: Liquid dispensing.

Type	PU	Cat. No.
Universal model, for pipettes up to 10 ml	1	104099
Universal model, for pipettes up to 100 ml	1	104199



Pipette fillers

For pipetting liquids, fit all glass and plastic pipettes. Slow rotation of the actuator-wheels draws liquid into the pipette. Pressing the air bleed valve automatically empties the pipette without returning the piston.

For pipettes ml	Colour	PU	Cat. No.
2	Blue	1	324594
10	Green	1	324694
25	Red	1	324794






Pipette stand, PP

Upper portion with 94 bore holes of different diameters for secure placement of volumetric and measuring pipettes of any size.

The stable base has a rotatable, ribbed base plate in which the pipette tips can be gently seated.

The racks are supplied unassembled, and can easily be assembled according to the accompanying assembly instructions.

Ø mm	Height mm	PU	Cat. No.
230	470	2	79194

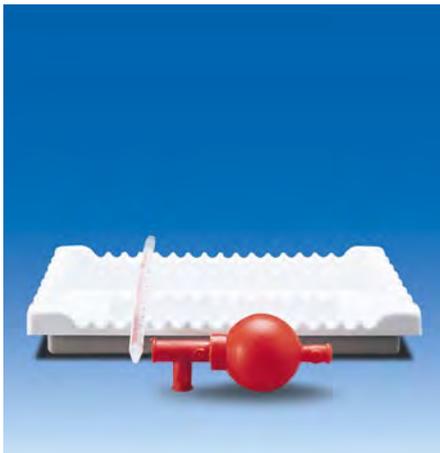

Pipette tray, PVC

Holds pipettes from 120 mm length.

Pipettes can easily be placed in and taken out from the troughs in the tray, even with gloves.

L x W x H mm	PU	Cat. No.
283 x 216 x 40	1	80996



Pipette tray, PVC

Suitable for drawers, divided lengthwise into 4 compartments.

L x W x H mm	PU	Cat. No.
420 x 300 x 30	1	80252

Volume measurement

Pipette washer, PE-HD

For simple and basic cleaning of pipettes. With discharge siphon for an automatic water exchange.

The complete washing system includes the pipette washer, pipette jar (for pre-cleaning) and pipette basket (for dipping pipettes into the pipette washer or pipette jar). Pipette jars and pipette baskets need to be ordered separately.

Suitable for the use with pipette baskets (cat. nos. 80219 and 80222).

Ø mm	Height mm	Effective length mm	PU	Cat. No.
170	734	600	1	80217
170	990	840	1	80215



Pipette jars, PE-HD

For pre-cleaning pipettes in detergent solutions.

Suitable for the use with pipette baskets (cat. nos. 80219 and 80222).

Ø mm	Height mm	PU	Cat. No.
125	250	1	80223
162	503	1	80221
162	650	1	80218



Pipette baskets, PE-HD

For dipping pipettes into the pipette jar or pipette-washer and for transferring pipettes. With the extension piece, the total height of the pipette basket (cat. no. 80219) increases from 650 to 870 mm.

Description	Ø mm	Overall height mm	Basket height mm	PU	Cat. No.
Pipette basket	145	648	300	1	80219
Pipette basket	145	497	300	1	80222
Extension piece for the handle (pipette basket 80219)				2	81219



Competence in Plastic Labware

MEASURING AND TRANSFERRING



VITLAB 
Competence in Labware



Graduated beakers, PP, raised blue scale



Highly transparent. With easily readable, raised, embossed blue scale, and stable, easy-grip handle. To preserve markings, do not clean at temperatures exceeding 60 °C. Conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving, we recommend the design with raised graduations (cat. nos. 440941 - 447941).

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
50	2	70	40	24	446081
100	2	80	50	24	447081
250	5	120	74	12	440081
500	10	140	92	12	441081
1000	20	181	117	6	442081
2000	50	213	152	6	443081
3000	50	242	172	6	444081
5000	100	270	204	6	445081



Graduated beakers, PP, raised scale



Highly transparent. With a raised scale and stable, easy-grip handle. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
50	2	70	40	24	446941
100	2	80	50	24	447941
250	5	120	74	12	440941
500	10	140	92	12	441941
1000	20	181	117	6	442941
2000	50	213	152	6	443941
3000	50	242	172	6	444941
5000	100	270	204	6	445941

Measuring and transferring

Graduated beakers, stackable, PP



Highly transparent. With stable handle and easily readable, printed black scale on both sides. Therefore, the volume is equally visible for left- and right handers.

To preserve markings, cleaning at no higher than 60 °C is recommended. For autoclaving we recommend the design with raised graduations (cat. nos. 440941 - 447941).



Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
250	5	115	75	12	480941
500	10	140	100	12	481941
1000	10	167	125	12	482941
2000	20	212	148	12	483941
3000	50	242	170	12	484941

Graduated beakers, stackable, coloured, PP



Graduated beakers in four different colours. Transparent, with stable handle and easily readable, printed scale on both sides. Therefore, the volume is equally visible for left- and right handers. To preserve markings, cleaning at no higher than 60 °C is recommended. For autoclaving we recommend the design with raised graduations (cat. nos. 440941 - 447941).



Volume ml	Colour	Divisions ml	Height mm	Ø mm	PU	Cat. No.
500	blue	10	140	100	12	481942
500	yellow	10	140	100	12	481943
500	red	10	140	100	12	481944
500	green	10	140	100	12	481945
500	Set: blue, yellow, red, green (1 item each)	10	140	100	1	4811111
1000	blue	10	167	125	12	482942
1000	yellow	10	167	125	12	482943
1000	red	10	167	125	12	482944
1000	green	10	167	125	12	482945
1000	Set: blue, yellow, red, green (1 item each)	10	167	125	1	4821111



Graduated beakers, SAN



Crystal clear.
With a raised scale and stable, easy-grip handle.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
250	5	120	70	12	44091
500	10	133	91	12	44191
1000	10	170	116	6	44291
2000	20	215	150	6	44391
3000	50	242	170	6	44491



Collectors, PP or SAN



With a raised scale. Volume: 2000 ml.
With stable, easy-grip handle and white PC lid.
Diameter: 150 mm; height: 220 mm.

Description	Divisions ml	PU	Cat. No.
SAN, raised scale (Picture 1)	20	6	97891
PP, raised scale	50	6	978941
PP, raised, blue embossed scale (Picture 2)	50	6	978081
Accessories for collectors			
Lid, PC		6	97791



Measuring and transferring

Buckets, PE-HD



White. Without spout. With division into 1 liter segments.
Stable handle with reinforcement in the middle for comfortable carrying.
Tightly closing, transparent lid made of PE-LD - please order separately.

Description	Volume l	Divisions l	Height mm	Ø mm	PU	Cat. No.
Bucket	5	1	240	250	1	96093
Bucket	10	1	300	290	1	96393
Lid	for 5 L				1	96293
Lid	for 10 L				1	96593



Buckets with spout, PP



Transparent. With division into 1 liter segments.
With stable handle and spout for easy emptying.
Highly resistant to chemicals.
Without lid.

Volume l	Divisions l	Height mm	Ø mm	PU	Cat. No.
12	1	330	310	1	96694
15	1	370	310	1	96794





Measuring scoops, PP



White. Also suitable as weighing scoops. With precision formed filling edge and comfortable, stable handle. Easily readable volume quantities on the upper side of the handle.

Volume ml	Length mm	PU	Cat. No.
2	60	12	39194
5	82	12	39294
10	100	12	39394
25	135	12	39494
50	160	12	39594
100	200	12	39694
250	260	6	39794
500	315	6	39894
1000	385	6	39994



Measuring scoops, coloured, PP



Measuring scoops in seven different colours. Also suitable as weighing scoops. With precision formed filling edge and comfortable, stable handle. Easily readable volume quantities on the upper side of the handle.

Volume ml	Colour	PU	Cat. No.
50	red	12	395940
50	blue	12	395950
100	red	12	396940
100	gray	12	396943
100	black	12	396944
100	yellow	12	396946
100	blue	12	396950
100	green	12	396952
100	bright blue	12	396955
250	red	12	397940
250	blue	12	397950
100	Set: white, red, grey, black, yellow, blue, green, bright blue (1 item each)	1	3961111

Measuring and transferring

Scoops, PE-HD



Conical in shape with tapered filling edge.

Volume ml	Length mm	Colour	PU	Cat. No.
15	115	natural	12	40093
25	135	natural	12	40193
65	185	natural	12	40293
110	215	natural	12	40393
150	250	natural	12	40493
350	310	natural	6	40593
750	350	natural	6	40693
750	350	blue	6	406950
750	350	black	6	406944
1250	400	natural	6	40793
1250	350	blue	6	407950
1250	350	black	6	407944





Spatula, PA

Glass-fibre reinforced. Double spatula or spatula spoon, with stable, easy to hold handle in the middle.


Description	Length mm	PU	Cat. No.
Double spatula	150	10	80594
Double spatula	180	10	80595
Spatula spoon	180	10	80596
Spatula spoon	210	10	80593



Stirring rod, PP

Spatula-shaped extension for effective manual stirring of small volumes.


Length mm	PU	Cat. No.
245	10	80828

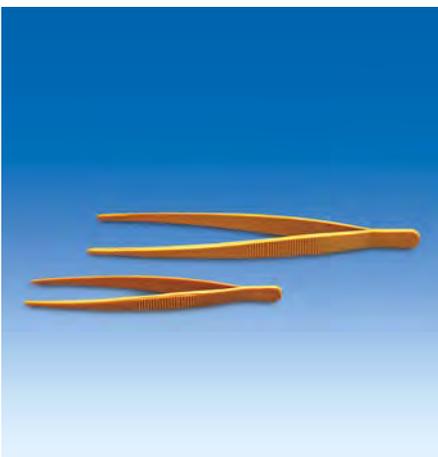

Forceps, POM

Yellow, blunt, elastic, very good resilience. With grooves on the outside for optimum handling and grip.

Length mm	PU	Cat. No.
115	5	68099
145	5	68199
180	5	68299
250	5	68399

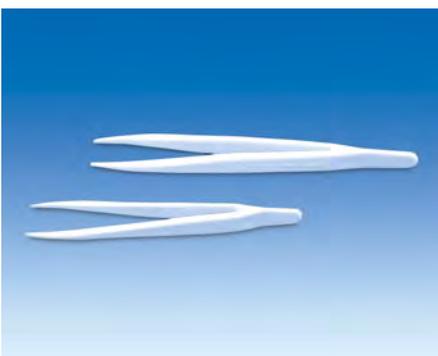

Forceps, PMP



White, pointed, elastic, very good resilience.

Length mm	PU	Cat. No.
115	10	67895
145	10	67995

Measuring and transferring

Funnels, PP



Transparent. Rapid flow due to a steep 60° angle.

Practical handle with loop for hanging.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	Stem length mm	PU	Cat. No.
5	30	45	1.5	25	24	40894
6	30	47	4	25	24	41094
14	40	65	4	35	24	41194
32	50	85	7	43	24	41294
88	75	110	6	55	12	41394
222	100	155	8	77	12	41494
342	120	180	11	90	12	41594
817	150	220	15	95	12	41694



Powder funnels, PP



Transparent. With short, wide stem. For transfer of powdered and granular substances.

Rapid flow due to a steep 60° angle.

Ø mm	Length mm	Inner stem Ø mm	Stem length mm	PU	Cat. No.
65	68	15	25	10	70794
80	75	21	25	10	70894
100	94	22	20	10	70994
120	110	26	20	10	71094
150	138	28	22	5	71194





Large funnels, PP



Transparent. Rapid flow due to a steep 60° angle. Practical handle for hanging. (Size 12500 ml without handle.) Suitable for filling large amounts of liquids. Optional accessories available: Stainless steel and aluminium sieve insert; however, not permissible for use with foodstuffs.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	PU	Cat. No.
1300	200	200	22	6	41794
3200	250	260	30	6	41894
12500	350	440	35	1	41994
Sieve insert Ø: 50 mm, for funnels no. 41794, 41894				1	42099



Large funnels, PE-HD

Transparent. Rapid flow due to a steep 60° angle. Practical handle for hanging. Suitable for filling large amounts of liquids.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	PU	Cat. No.
12500	400	365	42	1	42294
17500	430	420	37	1	42393



Standard joint funnels, PP



Transparent. For multi-neck flasks, laterally flattened, suitable for standard joint necks of various sizes. Suitable for the filling of liquid or powdered reagents into a reaction flask, especially for loading of multi-neck flasks during a reaction.

NS	Length mm	Wide opening mm	Stem length mm	PU	Cat. No.
14/23	75	40	17	10	70494
19/26	95	50	23	10	70594
29/32	135	75	30	5	70694

Competence in Plastic Labware

SAMPLE PREPARATION




VITLAB 
Competence in Labware

VITsafe™ - the Safety Wash Bottle


Working with chemical substances, which are sometimes dangerous, requires a high level of responsibility and concentration. With the VITsafe™ safety wash bottles VITLAB offers laboratory equipment that provides safety in the highest degree.

VENT-CAP virtually prevents leakage

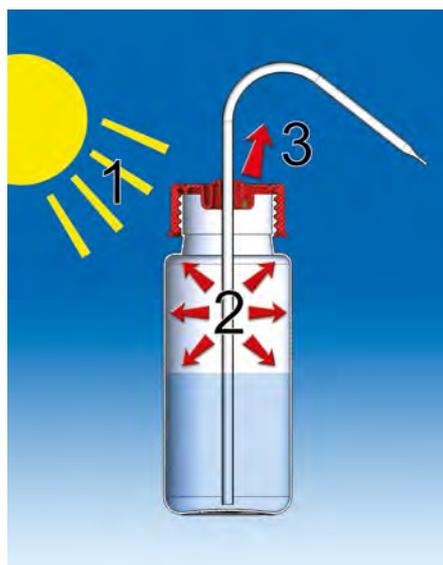

Temperature changes **(1)** in a laboratory can often cause conventional wash bottles to leak or drip due to the resulting increase in internal pressure **(2)**. The patent-registered, metal-free VENT-CAP screw closure of the VITsafe™ safety wash bottle virtually prevents this. The expansion of the gas due to the rise in pressure can escape through an integrated capillary **(3)**, thus dissipating the static over pressure. In addition, the lack of a spray insert allows turbulences to be almost completely avoided. The smooth and finely drawn tip of the spray bottle allows a precise spray jet and optimizes the fluid backflow. Dripping is subsequently almost entirely prevented.

Clear identification due to safety imprint

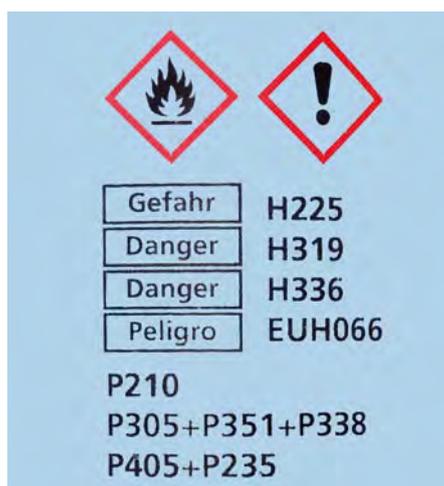

The permanent imprint according to directive (EC) No. 1272/2008 **(GHS)** offers even more safety.

It contains all essential information:

- Substance name in German, English, French and Spanish
- Chemical formula and CAS number
- Hazard pictogram with signal word
- Hazard (H) and precautionary (P) statements
- as well as the U.S.-based NFPA diamond

The VITsafe™ safety wash bottles are available as narrow-mouth or wide-mouth type. The particularly large opening of the wide-mouth bottles allows filling even without a funnel. Select the safety wash bottles to fit your applications from among **17 different substance names** and three volumes (250/500/1000 ml).

Sample preparation

VITsafe™ safety wash bottles, narrow-mouth



Bottles from PE-LD or PP, spray tube from PP.

More safety due to the durable safety imprint in accordance to Directive (EC) No. 1272/2008 (GHS), as well as with all important information:

- Material name in German, English, French and Spanish
- Chemical formula, CAS No., hazard pictogram, signal word
- Risk phrases (H phrases), safety phrases (P phrases), as well as NFPA Code

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube. Practically no leakage or dripping with the bright red VENT-CAP screw cap, the design of which prevents almost all static overpressure.



Imprint	Material	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
Acetone	PP	250	25	135	58	12	1431829
Acetone	PP	500	25	180	74	12	1432829
Acetone	PP	1000	32	215	92	12	1433829
Acetonitrile	PE-LD	500	25	180	74	6	1332969
Distilled Water	PE-LD	250	25	135	58	12	1331819
Distilled Water	PE-LD	500	25	180	74	12	1332819
Distilled Water	PE-LD	1000	32	221	92	12	1333819
Acetic acid	PE-LD	500	25	180	74	6	1332979
Ethanol	PE-LD	250	25	135	58	12	1331869
Ethanol	PE-LD	500	25	180	74	12	1332869
Ethanol	PE-LD	1000	32	221	92	12	1333869
Ethyl acetate	PE-LD	250	25	135	58	12	1331859
Ethyl acetate	PE-LD	500	25	180	74	12	1332859
Ethyl acetate	PE-LD	1000	32	221	92	12	1333859
Isopropanol	PE-LD	250	25	135	58	12	1331849
Isopropanol	PE-LD	500	25	180	74	12	1332849
Isopropanol	PE-LD	1000	32	221	92	12	1333849
Methanol	PE-LD	250	25	135	58	12	1331839
Methanol	PE-LD	500	25	180	74	12	1332839
Methanol	PE-LD	1000	32	221	92	12	1333839
Methylene chloride	PE-LD	500	25	180	74	6	1332879
Methyl ethyl ketone (MEK)	PP	500	25	180	74	6	1432989
Heptane	PE-LD	500	25	180	74	6	1332899
Hexane	PE-LD	500	25	180	74	6	1332909
N,N-Dimethylformamide	PE-LD	500	25	180	74	6	1332889
Pentane	PE-LD	500	25	180	74	6	1433959
Tetrahydrofuran (THF)	PE-LD	500	25	180	74	6	1332939
Toluene	PE-LD	500	25	180	74	6	1332949
Xylene	PE-LD	500	25	180	74	6	1332959

* Height without spray tube

Other variations available upon request.

→ VENT-CAP wash bottle caps can be found on page 69. →



VITsafe™ safety wash bottles, wide-mouth



Bottles from PE-LD or PP, spray tube from PP.

More safety due to the durable safety imprint in accordance to Directive (EC) No. 1272/2008 (GHS), as well as with all important information:

- Material name in German, English, French and Spanish
- chemical formula, CAS No., hazard pictogram, signal word
- Risk phrases (H phrases), safety phrases (P phrases), as well as NFPA Code

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube. Practically no leakage or dripping with the bright red VENT-CAP screw cap, the design of which prevents almost all static overpressure.

Imprint	Material	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
Acetone	PP	250	45	146	58	12	1451829
Acetone	PP	500	45	166	76	12	1452829
Acetone	PP	1000	63	226	91	12	1453829
Acetonitrile	PE-LD	500	45	166	76	6	1352969
Distilled Water	PE-LD	250	45	146	58	12	1351819
Distilled Water	PE-LD	500	45	166	76	12	1352819
Distilled Water	PE-LD	1000	63	226	91	12	1353819
Acetic acid	PE-LD	500	45	166	76	6	1352979
Ethanol	PE-LD	250	45	146	58	12	1351869
Ethanol	PE-LD	500	45	166	76	12	1352869
Ethanol	PE-LD	1000	63	226	91	12	1353869
Ethyl acetate	PE-LD	250	45	146	58	12	1351859
Ethyl acetate	PE-LD	500	45	166	76	12	1352859
Ethyl acetate	PE-LD	1000	63	226	91	12	1353859
Isopropanol	PE-LD	250	45	146	58	12	1351849
Isopropanol	PE-LD	500	45	166	76	12	1352849
Isopropanol	PE-LD	1000	63	226	91	12	1353849
Methanol	PE-LD	250	45	146	58	12	1351839
Methanol	PE-LD	500	45	166	76	12	1352839
Methanol	PE-LD	1000	63	226	91	12	1353839
Methylene chloride	PE-LD	500	45	166	76	6	1352879
Methyl ethyl ketone (MEK)	PP	500	45	166	76	6	1452989
Heptane	PE-LD	500	45	166	76	6	1352899
Hexane	PE-LD	500	45	166	76	6	1352909
N,N-Dimethylformamide	PE-LD	500	45	166	76	6	1352889
Pentane	PE-LD	500	45	166	76	6	1453959
Tetrahydrofuran (THF)	PE-LD	500	45	166	76	6	1352939
Toluene	PE-LD	500	45	166	76	6	1352949
Xylene	PE-LD	500	45	166	76	6	1352959

VENT-CAP wash bottle caps can be found on page 69.

* Height without spray tube

Other variations available upon request.

Sample preparation

VENT-CAP wash bottle caps, PP

Screw cap and spray tube from PP.

Practically no leakage or dripping with the bright red VENT-CAP screw cap, the design of which prevents almost all static overpressure.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Thread GL	PU	Cat. No.
25	12	833019
32	12	833029
45	12	833039
63	12	833049



Wash bottles with imprint, PE-LD/PP



Narrow- / wide-mouth bottles made of PE-LD, transparent.

Screw cap and spray tube from PP.

Imprinted with "Distilled Water" in German, English, French and Spanish.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Upon request, also with other imprints for non-hazardous media according to the REACH Directive.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	135	58	12	133181
250	45	146	58	12	135181
500	25	180	74	12	133281
500	45	166	76	12	135281
1000	32	221	92	12	133381
1000	63	226	91	12	135381

* Height without spray tube



Wash bottles made from PE-LD/PP with no imprint, transparent and coloured, can be found on page 71.



PFA-economy wash bottles



“PFA-economy” quality wash bottles. Transparent.

With recycled PFA content. Thus, reasonably priced and environmentally friendly.

PFA-economy bottles have excellent chemical resistance and high thermal stability from -200 °C to +260 °C and can be used for less critical applications for which pure PFA is not necessary.

Screw cap made from ETFE, spray tube from FEP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	157	61	1	108792
500	25	189	76	1	108892
1000	32	233	96	1	108992

* Height without spray tube



Wash-bottles, PP



Narrow- / wide-mouth bottles made of PP, transparent. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	135	58	12	94993
250	45	146	58	12	93793
500	25	180	74	12	95093
500	45	166	76	12	93993
1000	32	215	92	12	95193
1000	63	226	91	12	94193

* Height without spray tube

Sample preparation

Wash-bottles, PE-LD/PP



Narrow- / wide-mouth bottles made of PE-LD, transparent. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
50	18	73	37	24	94588
100	18	95	43	24	94688
250	25	135	58	12	94988
250	45	146	58	12	93788
500	25	180	74	12	95088
500	45	166	76	12	93988
1000	32	221	92	12	95188
1000	63	226	91	12	94188

* Height without spray tube



Wash bottles with imprint can be found on page 69.

Wash-bottles, coloured, PE-LD/PP

Narrow-mouth bottles, made from PE-LD. Available in four different colours to facilitate ready identification. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Colour	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
red	250	25	135	58	5	132603
red	500	25	180	74	5	132703
red	1000	32	221	92	5	132803
green	250	25	135	58	5	132605
green	500	25	180	74	5	132705
green	1000	32	221	92	5	132805
yellow	250	25	135	58	5	132606
yellow	500	25	180	74	5	132706
yellow	1000	32	221	92	5	132806
blue	250	25	135	58	5	132608
blue	500	25	180	74	5	132708
blue	1000	32	221	92	5	132808
Set: red, green, yellow, blue (1 item each)	500	25	180	74	1	1327111
Set: red, green, yellow, blue (1 item each)	1000	32	221	92	1	1328111

* Height without spray tube






Wash-bottles, PE-LD

Narrow-mouth bottles, transparent, with screw cap. Spray tube and spray-tube insert made from PE-LD. The classic model, made from soft material with good restoring force.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
100	18	106	45	50	134293
250	25	140	59	50	134393
500	25	180	75	50	134493
1000	28	212	94	25	134593

* Height without spray tube

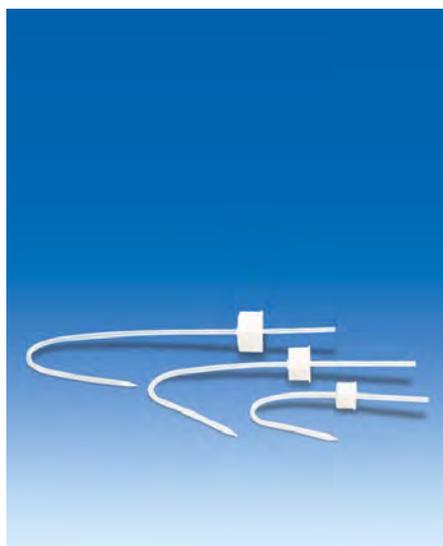

Wash bottle caps, PP

Screw cap and spray tube with drawn-out tip, made of PP. Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Thread GL	PU	Cat. No.
18	24	83300
25	12	83301
32	12	83302
45	12	83303
63	12	83304

Sample preparation

Dropping bottles, PE-LD/PE-HD



Narrow-mouth bottles made of PE-LD, transparent, with dropper insert and screw cap made from PE-HD.

Extra long, fine dropping tip for accurate dispensing.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	117	37	24	94587
100	18	142	43	24	94687
250	25	183	58	12	94987
500	25	228	74	12	95087
1000	32	269	92	12	95187



Caps with dropper inserts, PE-HD



For bottles with GL threads. Cap with dropper insert, complete with screw cap made from PE-HD.

Extra long, fine dropping tip for accurate dispensing.

Thread GL	PU	Cat. No.
18	24	83306
25	12	83307
32	12	83308




Dropping bottles, PE-LD

Narrow-mouth bottles, transparent, with dropper insert and red screw cap made of PE-LD. The classic model, made from soft material with good restoring force.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
20	14	88	31	100	132193
30	14	96	34	100	132293
50	18	115	39	100	132393
100	18	136	45	50	132493
250	25	170	59	50	132593
500	25	209	75	50	132693
1000	28	240	94	25	132793



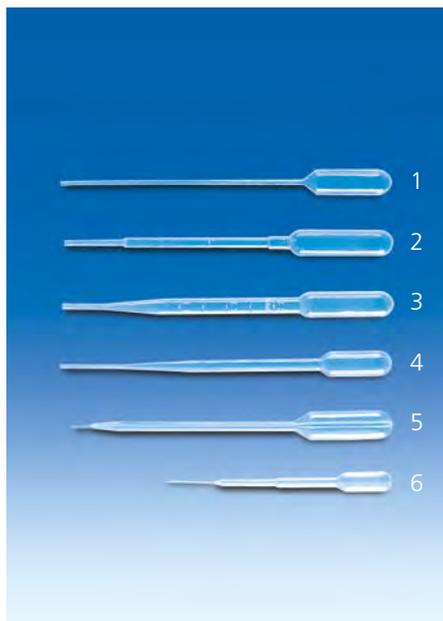

Pasteur pipettes, PE-LD

Disposable. Very good reproducibility of the number of drops per milliliter, thus ideal for distributing aliquots of liquid portions. Pasteur pipettes can be deep-frozen when filled, or if needed, be converted into sealed vessels through heat-sealing. The integrated suction bulb can readily be compressed. Thus, finger fatigue from frequent pipetting is avoided. Can be sterilised with gas or gamma radiation.

Figure No.	Graduations/ divisions ml	Max. suction volume ml	Tip outer Ø mm	Length mm	Number of drops per ml	PU	Cat. No.
1	-	3.0	2.8	152	25-27	5000	148893
2	1/0.25	3.5	3.4	151	25-30	5000	148993
3	3/0.5	3.5	3.2	152	21-28	5000	149093
4	2/0.5	2.0	3.3	152	22-26	5000	149193
5	-	4.0	1.0	148	52-65	5000	149293
6	-	1.0	1.0	105	50	3200	149393



Dropping pipettes, PE-LD

With integrated bellows.
For sampling and decanting of infectious or toxic liquids.
Graduated.

Volume ml	Length mm	PU	Cat. No.
1.5	134	100	149893
5	195	100	149993



Dropping pipettes, PE-LD

With integrated pipetting bulb.
For sampling and decanting of infectious or toxic liquids.
Without graduations.

Volume ml	Length mm	PU	Cat. No.
1.8	98	250	149693

Sample preparation

Spray bottles, PP

White or transparent bottles made from PP.

Sprayer insert with stable, smoothly operated pump trigger and adjustable spray nozzle, which can be regulated from the finest mist (nebulising) to a precise liquid jet.

Range: approx. 3-4 meters.

Ideal for spraying detergents or disinfectants, especially into difficultly accessible areas, as well as applications in thin layer chromatography.

Volume ml	Colour	PU	Cat. No.
400	white	5	53510
850	white	5	53610
1000	transparent	5	95286
1000	transparent with imprint „Ethanol“	5	952861





Griffin beakers, PFA



Transparent. With a raised scale. Excellent chemical resistance and very high thermal stability from -200 to +260 °C.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	32	1	110205
50	10	59	39	1	110305
100	20	72	50	1	110405
250	50	96	67	1	110605
500	100	122	88	1	110905
1000	100	141	109	1	111005

Watch glasses
can be found on page 80.

Sample preparation

Griffin beakers, ETFE



Transparent. With easily readable, printed black scale. According to ISO 7056.

Very good chemical resistance and very high thermal stability from -100 to +150 °C.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	32	1	110204
50	10	59	39	1	110304
100	20	72	50	1	110404
250	50	96	67	1	110604
400	50	109	77	1	110704
500	100	122	88	1	110904
600	100	125	91	1	110804
1000	100	143	105	1	111004



→ Watch glasses can be found on page 80. →

Griffin beakers, PTFE



White, opaque, thick-walled.

Without scale.

Excellent chemical resistance and high thermal stability from -200 to +260 °C.

Also suitable for microwave ovens.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Wall thickness mm	Height mm	Ø mm	PU	Cat. No.
5	2	26	20	1	112197
10	2	33	24	1	112297
25	2	47	32	1	112397
50	2	60	43	1	112497
100	3	68	54	1	112597
250	3	97	66	1	112697
500	4	125	80	1	112797
1000	4	155	100	1	112897





Griffin beakers, PMP, printed red scale

Crystal clear. With easily readable, printed red scale.

According to ISO 7056.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
10*	2	36	30	12	60503
25	5	50	38	12	60603
50	10	60	47	12	60703
100	10	70	55	12	60803
150*	20	80	66	12	60903
250	25	95	77	6	61003
400*	50	112	87	6	61103
500	50	118	94	6	61803
600*	50	127	100	6	61203
1000	100	147	120	6	61403
2000	200	187	149	6	61503
3000	250	212	170	4	61603
5000	500	247	203	4	61703

* Variant in addition to ISO 7056



Griffin beakers, PMP, raised scale

Crystal clear. With raised scale.

According to ISO 7056.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	38	12	60695
50	10	60	47	12	60795
100	10	70	55	12	60895
150*	20	80	66	12	60995
250	25	95	77	6	61095
400*	50	112	87	6	61195
500	50	118	94	6	61895
600*	50	127	100	6	61295
1000	100	147	120	6	61495
2000	200	187	149	6	61595
3000	250	212	170	4	61695
5000	500	247	203	4	61795

* Variant in addition to ISO 7056

Sample preparation

Griffin beakers, PP, raised blue scale



Highly transparent. With easily readable raised, embossed blue scale.
According to ISO 7056.

To preserve markings, do not clean at temperatures exceeding 60 °C.

Conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving we recommend the design with raised graduations (Cat. No. 606941 – 617941).



Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
10*	2	36	30	12	605081**
25	5	50	38	12	606081**
50	10	60	47	12	607081**
100	10	70	55	12	608081
150*	20	80	66	12	609081
250	25	95	77	6	610081
400*	50	112	87	6	611081
500	50	118	94	6	618081
600*	50	127	100	6	612081
1000	100	147	120	6	614081
2000	200	187	149	6	615081
3000	250	212	170	4	616081
5000	500	247	203	4	617081

* Variant in addition to ISO 7056

** Blue printed scale, not raised

Griffin beakers, PP, raised scale



Highly transparent. With raised scale.

According to ISO 7056.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	38	12	606941
50	10	60	47	12	607941
100	10	70	55	12	608941
150*	20	80	66	12	609941
250	25	95	77	6	610941
400*	50	112	87	6	611941
500	50	118	94	6	618941
600*	50	127	100	6	612941
1000	100	147	120	6	614941
2000	200	187	149	6	615941
3000	250	212	170	4	616941
5000	500	247	203	4	617941

* Variant in addition to ISO 7056





Measuring cup, PP

Transparent. With a raised scale. Volume: 30 ml; divisions: 1 ml.
Fitting lid made of PE - please order separately.
Diameter: 37 mm; height: 42 mm.

Description	PU	Cat. No.
Measuring cup	100	69394
Lid, PE	100	69493



Watch glasses, PTFE



White. Without base.
High thermal stability and chemical resistance.
Autoclavable at 121 °C (2 bar) according to DIN EN 285.
Ideal for use to cover beakers.

Ø mm	PU	Cat. No.
50	1	113197
75	1	113297
100	1	113397
125	1	113497



Watch glasses, PP



Transparent. With base.
Autoclavable at 121 °C (2 bar) according to DIN EN 285.
Ideal for use to cover beakers.

Ø mm	PU	Cat. No.
60	10	80452
80	10	80454
100	10	80455
125	10	80456

Sample preparation

Erlenmeyer flasks, PMP with PP screw cap



Transparent. Wide-mouth, can also be used with NS stoppers (not included).

Ideal for use as a receiving vessel in titrations.

Well suited for storage and cultivation of cell cultures. Far safer than glass flasks for use in incubator shakers due to the break resistance of plastic. Suitable for microwaves.

To preserve markings, cleaning at no higher than 60 °C is recommended.



Volume ml	Divisions ml	Thread GL	Neck NS	PU	Cat. No.
50	10	40	34/35	6	66695
100	20	40	34/35	6	66795
250	50	52	45/40	6	66895
500	100	52	45/40	6	66995
1000	200	52	45/40	4	67095

Erlenmeyer flasks, PP with PP screw cap



Transparent. Wide-mouth, can also be used with NS stoppers (not included).

Well suited for storage and cultivation of cell cultures. Far safer than glass flasks for use in incubator shakers due to the break resistance of plastic. Suitable for microwaves.

To preserve markings, cleaning at no higher than 60 °C is recommended.



Volume ml	Divisions ml	Thread GL	Neck NS	PU	Cat. No.
50	10	40	34/35	6	666941
100	20	40	34/35	6	667941
250	50	52	45/40	6	668941
500	100	52	45/40	6	669941
1000	200	52	45/40	4	670941

NS stoppers can be found on page 112.



Magnetic stirring bars, polygonal, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates.

Ø mm	Length mm	PU	Cat. No.
2	5	5	300497
2	7	5	300597
3	8	5	300897
3	10	5	301097
3	13	5	301197
4.5	12	10	301597
6	10	10	301697
6	15	10	301797
6	25	10	301997
6	30	10	302097
7	20	10	301897
7	50	10	302297
7	60	10	302397
8	40	10	302197
10	70	5	302497
10	80	5	302597
27	57	1	303097
27	108	1	303197
27	159	1	303297



Magnetic stirring bars, oval, PTFE



With permanent magnet AlNiCo V core. Highly suitable for vessels with a round bottom, such as round-bottom flasks. The angled side surfaces act to produce high turbulence, and thus achieve effective mixing.

Ø mm	Length mm	PU	Cat. No.
5	10	3	311097
6	15	3	311197
10	20	3	311297
12	25	3	311397
16	30	3	311497
16	35	3	311597
20	40	1	311697
20	50	1	311797

Sample preparation

Magnetic stirring bars, octagonal, PTFE



With rings and permanent magnet AlNiCo V core. The eight-sided shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates. The middle ring also promotes stable centering with convex or uneven bottoms.

Ø mm	Length mm	PU	Cat. No.
8	13	3	307697
8	15	3	307797
8	22	3	307897
8	25	3	307997
8	28	3	308097
8	38	3	308197
8	41	3	308297
8	51	3	308397
8	64	3	308497
10	13	3	308597
10	25	3	308897
10	35	3	308997
10	38	3	309097
10	51	3	309297
10	64	3	309397



Magnetic stirring bars, cross shape, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates. The cross shape promotes very stable centering.

Size mm	Height mm	PU	Cat. No.
10 x 10	5	1	316097
20 x 20	8	1	316197
25 x 25	9	1	316297
30 x 30	10	1	316397
38 x 38	11	1	316497





Magnetic stirring bars, triangular, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates.

Edges mm	Length mm	PU	Cat. No.
6	12	3	310197
8	25	3	310297
14	40	3	310397
12	50	3	310497



Magnetic stirring bars, barbell, PTFE



With permanent magnet AlNiCo V core. Excellent centering due to the small contact surface, and effective mixing. Disk diameter: 20 mm; shaft diameter: 8 mm.

Length mm	PU	Cat. No.
35	3	3125970
55	3	3126970




Magnetic stirring bar retrievers, flexible, PTFE



Flexible magnetic stir bar retriever with a total length of 330 mm. Magnet encapsulated. Ø x L 12.5 x 51 mm. Due to the high flexibility, the magnet stir bar can be retrieved from inaccessible locations, e.g., from the water trap in a laboratory sink. High chemical resistance, simple to clean.

Length mm	PU	Cat. No.
330	1	318597

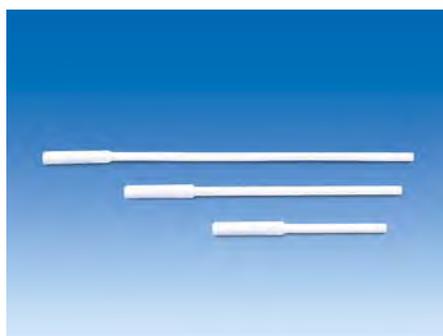

Magnetic stirring bar retrievers, PTFE



With PTFE encapsulated magnetic core. Straight shape. High chemical resistance, simple to clean.

Length mm	PU	Cat. No.
150	1	122097
250	1	122197
350	1	122297

Sample preparation

Magnetic stirring bar retrievers, PE



With a permanent magnet on one end and holding ring on the other one.
Magnet is completely encapsulated in a PE mantle.



Length mm	PU	Cat. No.
300	1	318293
450	1	318393

Mortars, MF

White, with spout. Stable circumferential edge. Very stable.

Volume ml	Height mm	Ø mm	PU	Cat. No.
300	75	125	5	72898
500	90	150	5	72998



Pestles, MF

White, heavy design. with ergonomically shaped grip.

Length mm	Head Ø mm	Weight g	PU	Cat. No.
125	30	55	5	73498
145	35	85	5	73598
160	40	120	5	73698
215	42	175	1	73898



Competence in Plastic Labware

MATERIAL SEPARATION



VITLAB 
Competence in Labware

Sample preparation – material separation

Urbanti funnels, PMP

Crystal clear. The spiral-shaped ribs increase the rate of filtration and prevent the trapping of air between the filter paper and the funnel. With long stem.

Volume approx. ml	Ø mm	Length mm	Stem Ø mm	Stem length mm	PU	Cat. No.
30	51	195	3	150	6	325095
80	70	210	3	150	6	325195
250	100	198	7	108	4	325295
630	140	247	10	132	3	325395
1800	196	315	20	155	2	325495



Analytical funnels, PP

Transparent. With long stem and grooves. Rigidified by a thickened edge. Rapid flow due to a steep 60° angle.

Volume approx. ml	Ø mm	Length mm	Stem Ø mm	Stem length mm	PU	Cat. No.
50	50	194	5	150	10	80162
100	72	208	5	143	10	80164
225	91	227	5	145	10	80165



Büchner funnels, PP

Three parts. Upper and lower parts are detachable to facilitate cleaning.

Volume approx. ml	Filter Ø mm	Length mm	Hole Ø mm	PU	Cat. No.
40	42.5	95	1.2	1	80437
70	55	113	1.1	1	80438
180	70	145	2.0	1	80439
280	80	165	2.0	1	80440
390	90	180	2.5	1	80441
810	110	210	2.5	1	80442
2100	160	280	2.75	1	80443
6000	240	350	3.0	1	80445



Water-jet pump, PP



For generation of a vacuum and to siphon off liquids and vapours (if necessary, with a suction main or condensation trap connected upstream).


Pump fluid: Water

Length of the unit: approx. 210 mm (R 3/4" connector fitted)

Weight: approx. 33 g (R 3/4" connector fitted)

- High chemical resistance, since the pumped media only come into contact with polypropylene, FKM and PTFE.
- Operating temperature up to a maximum of 80 °C.
- Integrated non-return valve increases operating safety.
- Simple operation, and easy to clean.
- Detachable vacuum connection.
- Variety of supplied adapters simplify connections to most water sources, and additional reducing adapters are available.

Water consumption as function of water supply pressure

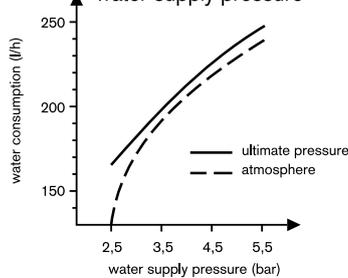


Very low water consumption:

The flow configuration has been optimised, resulting in a 33% reduction of water consumption (190 liters/h at 3.5 bar water supply pressure).

Constant discharge pressure:

The discharge pressure of 16 mbar (water temperature: 12 °C) is reachable across a wide range of water supply pressures of from 3 to 6 bar.

Ultimate pressure as function of water temperature

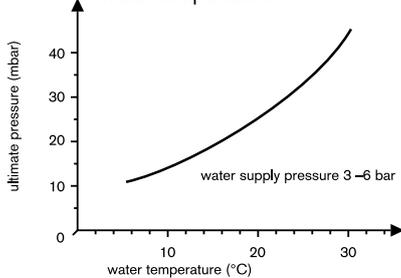


High suction capacity:

The suction capacity is approx. 400 L/hour of air (vs. atmospheric pressure, 12 °C water temperature, 3.5 bar water supply pressure).

Included in delivery:

Water jet pump, including: water supply connection (lock nut R 3/4", reducing adapter R 1/2" and hose connection (olive) with outer Ø 10-12 mm), vacuum connection (olive with outer Ø 6-9 mm, detachable with GL 14 screw cap).

Pumping capacity as function of back pressure

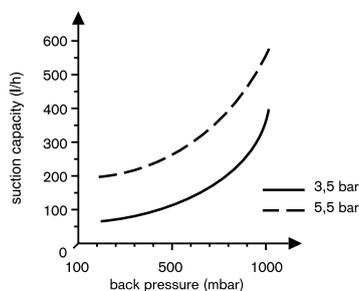

Description	PU	Cat. No.
Water-jet pump	1	77094
Accessories:		
Reducing adapter R3/4 inch to R3/8 inch	1	159665
Reducing adapter R3/4 inch to M 22x1, Perlator thread	1	159670

Sample preparation – material separation

Filtering racks

Funnel holder with base and adjustable height, made from PP, support stand made from aluminium, diameter: 12.7 mm; and, length: 595 mm. To hold from two to four funnels with an upper outer diameter of 50-120 mm.

Positions	Base plate mm	PU	Cat. No.
2	250 x 140	1	78394
4	450 x 140	1	78294



Support for separatory funnels, PP

For separatory funnels of from 125-500 ml. With practical clamps for simple attachment to stand rods with diameters of 8-14 mm.

Positions	PU	Cat. No.
1	5	80970





Imhoff or sedimentation cone, SAN



According to DIN 12 672. Crystal clear, with raised scale for precise reading of volumes. For simple, basic cleaning and rinsing, the screw coupling on the tip can be removed. Lower breakage risk than for PC or glass containers. For determination of suspended matter in liquids (e.g., for industrial and municipal wastewater).

Graduation:	Divisions:	Error limits:
0 - 2 ml	0.1 ml	+/- 0.1 ml
2 - 10 ml	0.5 ml	+/- 0.5 ml
10 - 40 ml	1 ml	+/- 1 ml
40 - 100 ml	2 ml	+/- 2 ml
100 - 1000 ml	50 ml	+/- 10 ml

Volume ml	PU	Cat. No.
1000	3	75991



Sedimentation rack, PMMA

Holds two Imhoff sedimentation cones. Base plate with depression for exact vertical positioning of the sedimentation cone.

L x W x H mm	PU	Cat. No.
150 x 300 x 290	1	81056



Evaporating dishes, PFA



With snap-on lid, PE. For contamination free sample preparation and efficient transportation. Due to a conical depression in the middle of the base very small amounts of a solvent are adequate to absorb the evaporated samples.

Volume ml	Height mm	Ø mm	PU	Cat. No.
25	25	50	1	103297
50	54	50	1	103397

Sample preparation – material separation

Round-bottom flasks, PFA



Transparent, neck with NS 29/32. Suitable as safety flask for use with rotary evaporators (operation at room temperature) to collect the distilled off liquid. High thermal stability and chemical resistance.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable.
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Height mm	Ø mm	PU	Cat. No.
100	117	65	1	107797
250	147	88	1	107897
500	177	107	1	107997



Round-bottom flask stand, PP



White, for flasks with a round bottom. Excellent chemical resistance. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Ø mm	PU	Cat. No.
160	5	80271





Gas wash bottles, PFA



Cap with S 40 buttress threads, and frit made of PTFE. A pore size of approx. 50 μm for optimal optimal pearling of the gas into the liquid. A wide field of application is possible due to the use of high-quality fluoroplastic. Suitable only for non-pressurised operation.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Height mm	Ø mm	Hose connection inner / outer Ø mm	PU	Cat. No.
250	160	61	4 / 6	1	159497
500	190	76	4 / 6	1	159597
1000	240	96	5 / 8	1	159697

Sample preparation – material separation

Desiccators with stopcock, PC

Crystal clear, with stopcock for evacuation. Lower sections can be filled with desiccants. The materials to be dried are placed on a perforated disc made of PP. Lid is sealed by a neoprene gasket. Ideal for use in educational laboratories.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
171	140	206	1	326496
230	190	260	1	326596
273	230	311	1	326696



Desiccators, PP/PC

Lower portion made from PP can be filled with desiccants. The materials to be dried are placed on a perforated disc made of PP. The lid made from PC is sealed with a neoprene gasket. Ideal for use in educational laboratories.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
171	140	206	1	326094
230	190	260	1	326194
273	230	311	1	326294



Desiccators with stopcock, PP/PC

With a bleed valve and an O-ring seal between the dome and the lower portion. The desiccators are suitable for vacuum and are provided with a non-return valve. Hot crucibles should only be placed on a porcelain plate, and should not come into too close contact with the rim of the desiccator. The insert made of PP serves to hold the drying agent. Desiccator plates should be purchased separately.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
150	140.5	190	1	80550
200	189	230	1	80230
250	238	300	1	80554



Desiccator plates, PP and porcelain



PP plate, usable up to a max. of 120 °C. Porcelain plates are suitable for hot objects.

Material	For desiccator Ø mm	Ø mm	PU	Cat. No.
PP	150	140.5	1	80551
PP	200	189	1	80231
PP	250	238	1	80553
Porcelain	150	140	1	65965
Porcelain	200	190	1	65975
Porcelain	250	235	1	65980

Replacement parts for desiccators



Replacement O-rings and valves for desiccators (cat. nos. 80550, 80230, 80554).

Description	PU	Cat. No.
O-ring for desiccator no. 80550	1	80555
O-ring for desiccator no. 80230	1	80556
O-ring for desiccator no. 80554	1	80557
Valve, PC, for desiccator nos. 80550, 80230 and 80554	1	80229

Sample preparation – material separation

Sample containers, PFA



With screw cap made of PFA. Cylindrical, tall shape.
Ideal for sample collection, transport and storage of samples.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability from -200 °C to +260 °C, autoclavable at 121 °C (2 bar) according to DIN EN 285
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw material

Further information on PFA can be found starting on page 130.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
30	40	54	38	1	130297
60	40	90	38	1	130397
90	56	62	54	1	130497
180	56	112	54	1	130597



Sample containers, PE-HD

With screw cap made of PE-HD. Cylindrical, tall shape.
Ideal for sample collection, transport and storage of samples.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
5	23	36	21	10	80910
10	23	58	21	10	80911





Sample containers, PP



Transparent. With screw cap made of PP. Cylindrical, tall shape.
Ideal for sample collection, transport and storage of samples.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
30	40	54	38	10	130294
60	40	90	38	10	130394
90	56	62	54	10	130494
180	56	112	54	10	130594



Sample containers, PP



Transparent. With snap-on lid made of PE-LD. Conical shape.

Volume ml	Height mm	Ø mm	PU	Cat. No.
5	25	20	25	68594
18	57	22	25	68894
50	97	30	10	69194
160	110	50	10	69294



Sample containers, PE-LD

Transparent. With attached snap-on lid made of PE-LD.

Volume ml	Height mm	Ø mm	PU	Cat. No.
1	32	9	500	80730
2	32	14	100	80731
5	50	15	100	80737
8	56	17	100	80732
10	32	22	100	80733
25	72	24	100	80734
30	52	31	50	80736
50	74	30	50	80735

Sample preparation – material separation

Weighing jars, PP

Transparent. With knobbed lid. Cylindrical shape.

Volume ml	Height mm	Ø mm	PU	Cat. No.
25	30	40	10	80342
30	50	30	10	80340
50	30	50	10	80345
65	35	60	10	80346
65	60	40	10	80343
200	90	60	10	80347
400	120	70	10	80348



Sample tubes, PFA



Sample tubes made from PFA for sample preparation, centrifugation and for use in autosampler racks. With or without individually calibrated ring mark at 10 ml with GL 25 screw cap made from PFA or PE stopper (see Table).

The advantages of PFA:

- Especially suitable for use in trace analysis
- No memory effects
- Practically no carryover due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean

Further information on PFA can be found starting on page 130.

Figure Type No.		Volume ml	Height mm	Ø mm	PU	Cat. No.
1	With ring mark and screw cap	15	110	22	1	103897
-	Without ring mark	15	110	22	1	1038971
2	With ring mark and stopper	12	110	16	1	1037979
3	Without ring mark	12	110	16	1	103797





Sample vials, PFA



Sample vials made of PFA with conical interior and raised graduation (5 ml subdivisions). Available in two different types, depending on application:

- Cored outside bottom
- Flat surface on bottom of vial for improved heat transfer (Recommended for use with hot plates)

Both 50 ml sizes fit in common Autosampler racks.

Scope of delivery is without screw cap. Please order the screw cap (Cat. No. 104997) separately.

Volume ml	Type outside bottom	Outer-Ø mm	Height* mm	PU	Cat. No.
15	Flat	29	39	1	104197
15	Cored	29	42	1	104097
25	Flat	29	69	1	104397
25	Cored	29	72	1	104297
50	Flat	29	117	1	104597
50	Cored	29	120	1	104497
Screw cap, 33 mm, PFA (suitable for sample vials (104097 – 104597))				1	104997

* Height with thread



Autosampler-vials, PFA




Raised graduation with 1 ml subdivisions.

Translucent material for optimum visibility of the liquid contained in the vial.

Conical interior for use with autosamplers. The outer design allows easy handling of the autosampler-vials with forceps. Optionally available with snap cap for long term storage or lid with knob for fast opening and closing (dust protection) of the vial.

Scope of delivery is without lid or cap. Please order the fitting lid (Cat. No. 105597 resp. 105697) separately.

Volume ml	Outer-Ø mm	Height mm	PU	Cat. No.
1.5	13.5	24	1	105097
2.5	13.5	36	1	105197
4	14	52	1	105297
Snap cap, PFA		18	5	105697
Lid with knob, PFA		16	9	105597

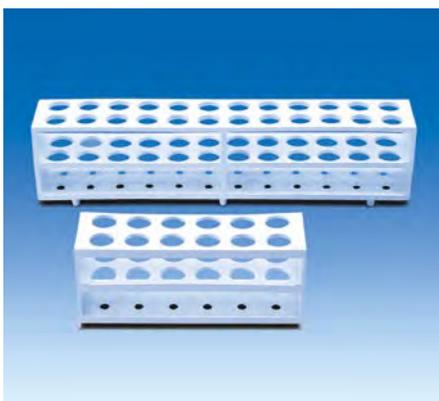

Reagent tube racks, PP



White. For reagent tubes with a diameter of 21 mm.

With three levels for precise, vertical positioning of the reagent tubes.

Working temperatures of -20 to +90 °C.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

For Ø up to mm	Positions	L x W x H mm	PU	Cat. No.
21	2 x 6	190 x 60 x 80	5	80560
21	2 x 12	375 x 65 x 85	5	80562

Sample preparation – material separation

Reagent tube racks, PP

White. The special shape makes it possible to check the amounts present in the reagent tubes.

With two side-mounted handle straps.

For Ø up to mm	Positions	L x W x H mm	PU	Cat. No.
16	10	200 x 55 x 65	4	80130
18	9	200 x 55 x 65	4	80131
Base plate for 2 reagent tube racks		202x156x13.5	4	80134
(Cat. No. 80130, 80131)				



Test tube racks, coloured, PP



Stackable, simple, and small footprint. Alphanumerically identified positions. Suitable for tempering in a water bath as well as storage of samples in the refrigerator and incubation in a climate chamber. The racks are supplied as folded out flat, and can be firmly and inseparably joined together in just a few steps. Working temperatures of -20 to +90 °C. Autoclavable at 121 °C (2 bar) according to DIN EN 285. Base area: 265 x 126 mm.

For Ø up to mm	Positions	Height mm	Colour	PU	Cat. No.
13	6 x 14	75	White	5	3190940
16	5 x 11	75	White	5	3191940
18	5 x 11	75	White	5	3192940
20	4 x 10	75	White	5	3193940
25	4 x 8	88	White	5	3194940
30	3 x 7	88	White	5	3195940
13	6 x 14	75	Blue	5	3190948
16	5 x 11	75	Blue	5	3191948
18	5 x 11	75	Blue	5	3192948
20	4 x 10	75	Blue	5	3193948
25	4 x 8	88	Blue	5	3194948
30	3 x 7	88	Blue	5	3195948
13	6 x 14	75	Red	5	3190943
16	5 x 11	75	Red	5	3191943
18	5 x 11	75	Red	5	3192943
20	4 x 10	75	Red	5	3193943
25	4 x 8	88	Red	5	3194943
30	3 x 7	88	Red	5	3195943





Microtubes, PP



With lid, with frosted labelling field. Raised graduations for reading the volume. The lid membrane has a uniform thickness and can be easily pierced by an analyzer. The attached lid seals tightly and is firmly seated, yet reopens easily. The microtubes have a uniform wall thickness and are highly transparent. CE marked according to IVD Directive 98/79 EC.

- Can be centrifuged at an RCA of up to 20,000 RCF at 20 °C for up to 20 min
- Lid membrane Ø: 8.5 mm; approx. 0.3 mm thick
- Outer Ø x H: 10.75 x 40.8 mm

Volume ml	Packaging units	PU	Cat. No.
1.5	1x500	500	145094
1.5	6x500	3000	145194



Microtube stands, PP



Opaque, gray. Numbered positions for 20 microtubes with volume of 1.5 ml. For working with samples as well as short- and medium-term storage. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Positions	L x W x H mm	PU	Cat. No.
20	210 x 70 x 37	1	3190941



Microtube racks, coloured, PP



Stackable racks for micro- or cryotubes. Alphanumerically identified positions. Suitable for tempering in a water bath. The racks are supplied as folded out flat, and can be firmly and inseparably joined together in just a few steps. Working temperatures of -20 to +90 °C. Autoclavable at 121 °C (2 bar) according to DIN EN 285. Base area: 265 x 126 mm.


For Ø up to mm	Positions	Colour	Height mm	PU	Cat. No.
11	8 x 16	White	38	5	3197940
13	6 x 14	White	38	5	3198940
11	8 x 16	Blue	38	5	3197948
13	6 x 14	Blue	38	5	3198948
11	8 x 16	Red	38	5	3197943
13	6 x 14	Red	38	5	3198943

Sample preparation – material separation

Staining chamber for slides, POM

Consists of staining jar and a staining rack for 25 slides 76 x 26 mm.

L x W x H mm	PU	Cat. No.
100 x 87 x 51	5	99099

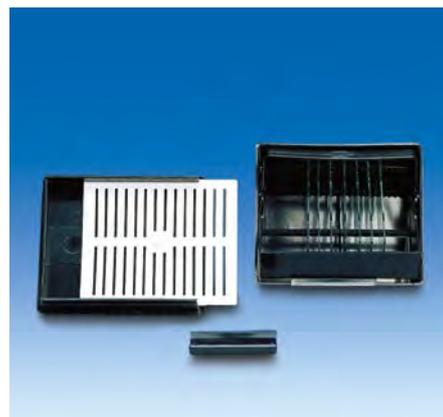

Staining rack for slides, POM

For serial staining of 25 slides 76 x 26 mm.
Usable in the staining jar, cat. no. 99199. (see below).

L x W x H mm	PU	Cat. No.
91 x 79 x 38	10	99299



Staining jar for slides, POM

For combination with staining rack, cat. no. 99299 (see above).
Can also be used as a storage box for 25 slides.

L x W x H mm	PU	Cat. No.
100 x 87 x 51	5	99199



Slide storage boxes, PS

With lid. For 25, 50 or 100 slides, 76 x 26 mm. Handy, stackable, break resistant, easy to clean. The positions are numbered individually. With an index card.

Positions	L x W x H mm	PU	Cat. No.
25	122 x 96 x 34	4	80276
50	229 x 96 x 34	1	80277
100	229 x 181 x 34	1	80278



Coplin staining chamber, PP

With screw top. For serial staining of 10 slides 76 x 26 mm.



Height mm	Screw cap outer Ø mm	Inner Ø mm	PU	Cat. No.
94	50	34	10	136693

Competence in Plastic Labware

SAVING AND STORAGE WITH CONFIDENCE



VITLAB [®]
Competence in Labware



Narrow-mouth bottles, PFA



Transparent.

With screw cap with buttress threads made of PFA. Ideal for long-term storage of high-purity oxidants, acids, alkalis, as well as hydrocarbons, trace analysis solvents and standards.

Volume ml	Thread	Height mm	Ø mm	PU	Cat. No.
50	S 28	86	37	1	109297
100	S 28	120	45	1	109397
250	S 28	160	61	1	108297
500	S 28	190	76	1	108397
1000	S 28	240	96	1	108497

The advantages of PFA:

- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.



Wide-mouth bottles, PFA



Transparent.

With screw cap made of PFA with buttress threads. Ideal for long-term storage of high-purity oxidants, acids, alkalis, as well as hydrocarbons, trace analysis solvents and standards.

Volume ml	Thread	Height mm	Ø mm	PU	Cat. No.
250	S 40	150	61	1	109497
500	S 40	179	76	1	109597
1000	S 40	217	96	1	109697
2000	S 40	245	130	1	109797

Saving and storing

PFA-economy narrow-mouth bottles



Narrow-mouth, "PFA-economy" quality wash bottles. Transparent.
With recycled PFA content. Thus, reasonably priced and environmentally friendly.
PFA-economy bottles have excellent chemical resistance and high thermal stability from -200 °C to +260 °C and can be used for less critical applications for which pure PFA is not necessary.
With screw cap made of ETFE.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	90	37	1	108092
100	18	114	45	1	108192
250	25	157	61	1	108292
500	25	189	76	1	108392
1000	32	233	96	1	108492



Screw caps, PFA



Transparent. For sealing all PFA containers with GL threads or buttress threads.
Autoclavable at 121 °C (2 bar) according to DIN EN 285.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Highly pure starting materials used

Further information on PFA can be found starting on page 130.

Thread	PU	Cat. No.
GL 18	1	102597
GL 25	1	102397
S 28	1	102697
S 40	1	102897





Wide-mouth bottles, PTFE



White. Opaque. Thick walled.
 With screw cap made of PTFE.
 Very high thermal stability and chemical resistance.
 With very wide mouth, ideal for filling with powders and paste-like materials.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
10	12	50	26	1	122597
25	19	61	33	1	122697
50	25	76	43	1	122797
100	35	88	52	1	122897



Narrow-mouth bottles, PP



Transparent. With high shoulders.
 With screw cap made of PP.
 Good chemical resistance, ideal for long-term storage of liquids.
 Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
250	25	135	58	12	94994
500	25	180	74	12	95094
1000	32	215	92	12	95194



Wide-mouth bottles, PP



Transparent.
 With screw cap made of PP.
 Good chemical resistance, ideal for long-term storage of liquids.
 Autoclavable at 121 °C (2 bar) according to DIN EN 285.
 Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
250	45	146	58	12	93794
500	45	166	76	12	93994
1000	63	226	91	12	94194

Saving and storing

Narrow-mouth bottles, PE-LD



Transparent. With high shoulders.

With screw cap made of PP.

Flexible material with good resilience.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	73	37	24	94589
100	18	95	43	24	94689
250	25	135	58	12	94989
500	25	180	74	12	95089
1000	32	221	92	12	95189



Wide-mouth bottles, PE-LD



Transparent.

With screw cap made of PP.

Flexible material with good resilience.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	32	87	39	24	93389
100	32	94	47	24	93489
250	45	146	58	12	93789
500	45	166	76	12	93989
1000	63	226	91	12	94189



Screw caps, PP



Transparent. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Thread GL	PU	Cat. No.
18	24	83310
25	12	83311
32	12	83312
40	12	83315
45	12	83313
52	12	83316
56	12	83317
63	12	83314





Narrow-mouth bottles, PE-LD

Transparent. With flat shoulders.
With screw cap made of PE-LD.
Flexible material with good resilience.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
10	14	50	26	100	138093
20	14	58	31	100	138193
30	14	66	34	100	138293
50	18	85	39	100	138393
100	18	106	45	50	138493
250	25	140	59	50	138593
500	25	180	75	50	138693
1000	28	212	94	25	138793
2000	28	264	117	25	138893



Wide-mouth bottles, PE-LD

Transparent.
With screw cap made of PE-LD.
Flexible material with good resilience.
Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	32	80	38	100	139393
100	32	94	48	50	139493
250	40	126	62	50	139593
500	50	155	76	50	139693
1000	65	208	93	25	139793
2000	65	246	120	25	139893

Saving and storing

Narrow-mouth bottles, PE-HD

Transparent.

With screw cap made of PP.

Small footprint due to the square cross-section and the high shoulders.

Volume ml	Thread GL	Height mm	Size mm	Mouth inner Ø mm	PU	Cat. No.
100	25	76	43 x 43	17.5	24	91789
250	28	80	80 x 80	21	24	91989
500	32	106	90 x 90	24	12	92089
1000	32	187	80 x 80	24	12	92189



Wide-mouth bottles, PE-HD

Transparent.

With screw cap made of PP.

Small footprint due to the square cross-section and the high shoulders.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Size mm	PU	Cat. No.
100	32	78	46 x 46	24	92489
250	50	83	80 x 80	24	92689
500	65	120	90 x 90	12	92789
1000	65	168	90 x 90	12	92889



Wide-mouth bottles, PE-LD, with eye closure

Transparent.

With eyes on the bottle and the screw cap for sealing.

With sealing plug and screw cap made of PE-LD.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
50	24	75	40	25	80408
100	24	90	50	25	80409
250	36	130	60	25	80410
500	36	160	75	10	80411
1000	50	200	95	10	80412
2000	50	250	115	10	80413





Reagent bottles, PP



Transparent.

With screw cap made of PP.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Size: 10,000 ml, with two handles.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
100	18	100	52	20	100389
100	32	96	55	20	101589
250	25	132	70	20	100489
500	25	165	87	10	100589
1000	32	202	108	10	100689
1000	63	204	108	10	101889
2000	32	245	131	6	100789
2000	63	243	131	6	101989
10000*	63	394	222	1	100989

* with PE foam seal



Reagent bottles, PP, GL 45



Transparent.

With screw cap made of PP.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
250	45	132	73	20	101689
500	45	172	87	10	101789
1000	45	197	105	10	102089
2000	45	241	131	6	102189
5000*	45	315	178	1	100889

* with handle

Saving and storing

Reagent bottles, PP



Transparent.

With NS stopper made of PP.

Stopper type A: With square-knob cap and red core.

Stopper type B: With hexagonal-knob cap and red core.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Neck NS	Height mm	Ø mm	Stopper	PU	Cat. No.
100	14/23	106	52	A	20	100394
100	29/32	111	55	B	20	101594
250	19/26	138	70	A	20	100494
250	34/35	144	73	B	20	101694
500	24/29	172	87	A	10	100594
500	45/40	183	87	B	10	101794
1000	29/32	213	108	A	10	100694
1000	60/46	214	108	B	10	101894



Reagent bottles, opaque, PP, wide mouth



Transparent. Made from opaque, pigmented PP for light-sensitive substances.

According to DIN 12039.

With NS stopper made of PP.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Further information on our opaque products can be found on page 132.

Volume ml	Neck NS	Height mm	Ø mm	PU	Cat. No.
500	45/40	183	87	10	1017940
1000	60/46	214	108	10	1018940
2000	60/46	263	131	6	1019940



VITLAB® opaque replaces brown glass and is...

- ... substantially lighter in weight
- ... practically unbreakable
- ... practically impermeable in the UV region
- ... comparable to a light protection factor of 20



Standard joint stoppers, PP



Stopper type A: With square-knob cap and red core.

Stopper type B: With hexagonal-knob cap and red core.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

NS	Model	PU	Cat. No.
10/19	A	1	90694
12/21	A	1	90794
14/23	A	1	90894
19/26	A	1	90994
24/29	A	1	91094
29/32	A	1	91194
29/32	B	1	92194
34/35	B	1	91294
45/40	B	1	91394
60/46	B	1	91494

Saving and storing

Storage bottles, PE-HD, without tap

Transparent.

With stable carrying handle and screw cap.

Available in wide- and narrow-mouth models.

Volume l	Thread mm	Height mm	Ø mm	PU	Cat. No.
5	94	340	170	1	81640
5	62.5	345	170	1	81644
10	108	415	210	1	81642
10	62.5	425	210	1	81646



Storage bottles, PE-HD, with tap

Transparent. Narrow-mouth model.

With stable carrying handle and screw cap. The 25 and 50 l sizes come equipped with two carrying handles.

Complete with exchangeable, easily operated tap made from PP with a 3/4" pipe fitting.

Volume l	Thread mm	Height mm	Ø mm	PU	Cat. No.
5	62.5	345	170	1	81660
10	62.5	425	210	1	81662
25	95.5	565	280	1	81664
50	95.5	700	350	1	81666



Tap for storage bottles, PP

Replacement tap for storage bottles made from PP (Cat. No. 81660 to 81666).

Complete with 3/4" pipe fitting and rubber ring.

Description	PU	Cat. No.
Tap for storage bottles	1	80375





Container, PP

Ideal for low-footprint storage of media. The rectangular shape means that the containers can be lined up side by side with no wasted space. Each container is supplied with a scale. With a wide opening for filling. Comfortable, simple dispensing of media with the easily operated dispensing and discharge tap. Dripping is prevented with the rotatable spout. Container supplied without stopcock.

Capacity 6 L

Measurements 65 x 335 x 335 mm

Filling opening diameter: 41 mm

Description	PU	Cat. No.
Rectangular carboy	10	155094
Vented screw cap	1	155594
Filling tap	1	156094



Chemical waste disposal system, PE/PP

For collection of liquid chemicals in the laboratory. The inlet hopper made from PE-HD contains a self-closing float, overfill protection, and a splash guard. Additionally, a screw cap (GL 63) with sealing ring is included.

Volume l	Height mm	Ø mm	PU	Cat. No.
10	560	222	1	151594

Saving and storing

Bowl, PP, with lid



White. Rectangular shape.

Broad, stable, easy to grip edge.

Especially easy to clean due to the rounded corners and edges and the smooth surfaces.

Volume l	L x W x H mm	PU	Cat. No.
17	430 x 331 x 195	1	43610



Transport containers, PE-HD

Transparent.

Easy stackable.

With reinforcing ribs and integrated carrying handles.

Broad, stable edge.

Volume l	L x W x H mm	PU	Cat. No.
20	380 x 280 x 200	1	80602
46	560 x 330 x 250	1	80603
72	660 x 400 x 300	1	80604



Multi-purpose container, SAN

Crystal clear, with fitted lid. Planar bottom inside, reinforced edge outside for stable placement on the lab bench.

Ideal for dust-proof storage of small components, instruments and utensils.

Volume ml	L x W x H mm	PU	Cat. No.
4000	340 x 230 x 94	1	36491





Dishes, PVC

White. All-purpose. Rounded corners and edges. Easy to clean.

Inner bottom dimensions mm	Height mm	PU	Cat. No.
200 x 150	50	1	80280
250 x 200	60	1	80281
320 x 260	70	1	80282
350 x 300	85	1	80283
430 x 330	95	1	80284
520 x 420	95	1	80285
675 x 540	100	1	80286
550 x 430	190	1	80288



Laboratory trays / catchment trays, PP



White. All-purpose. Robust design. Very good chemical resistance
Rounded corners and edges. Smooth surfaces, easy to clean.

Inner bottom dimensions mm	Edge dimensions mm	Height mm	PU	Cat. No.
130 x 180	180 x 230	42	1	165094
180 x 240	250 x 310	65	1	165194
240 x 300	310 x 370	75	1	165294
300 x 400	420 x 520	120	1	165394
400 x 500	534 x 634	140	1	165494
500 x 700	648 x 846	160	1	165594



Bowls, PP



White. Round. With broad, stable edge and circumferential standing ring on the bottom.


Volume l	Height mm	Ø mm	PU	Cat. No.
1	70	160	5	42594
2	80	200	5	42694
3	100	240	5	42794
4	120	280	5	42894
7	130	320	3	42994
9	150	360	3	43094
13	180	400	3	43194

Competence in Plastic Labware

LAB ASSISTANTS




VITLAB 
Competence in Labware

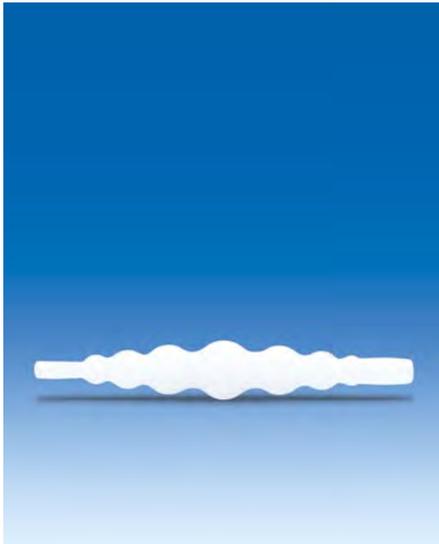

Connectors, universal, PP

Due to its special shape, it can be used for a wide variety of different tubing inner diameters.

For tubing with an inner Ø of mm	PU	Cat. No.
5 - 15	10	78794

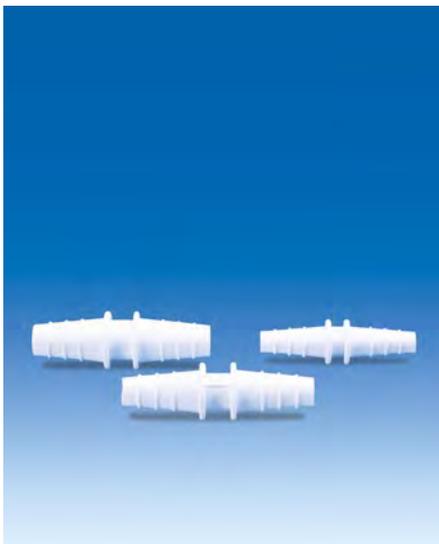

Connectors, straight, PP

Conical shape to accept tubing of various inner diameters.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3 - 5	2.0	20	80510
5 - 7	3.5	20	80511
7 - 10	4.5	20	80512
9 - 12	6.5	20	80513
11 - 14	8.5	20	80514
13 - 16	10.5	20	80515



Connectors, straight, PP

Conical shape, stepped. With different fitting diameters on the two sides to be able to connect with tubing having different diameters.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
4 - 8 / 8 - 12	1.6 / 4.6	20	80877
4 - 8 / 12 - 16	1.6 / 7.6	20	80878
8 - 12 / 12 - 16	4.6 / 7.5	20	80879

Lab assistants

2-way connectors, PE-HD

For connecting tubing of varying diameters. The connectors can be joined together with the next size up. Not suitable for pressure applications!

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3 - 5	1.6	20	80434
5 - 7	2.7	20	80435
7 - 9	3.6	20	80436
9 - 12	5.5	20	80535
11 - 14	7.3	20	80536
13 - 16	8.8	20	80537



Connectors, T-shape, PP



For the splitting or combining of liquid lines in a tubing system.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3	1.6	20	80459
4 - 5	3.7	20	80460
6 - 7	4.4	20	80461
8 - 9	6.3	20	80462
10 - 11	8.2	20	80463
12 - 13	10.0	20	80520
14 - 15	12.1	20	80521



Connectors, Y-shape, PP



For the splitting or combining of liquid lines in a tubing system.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3	2.0	20	80464
4 - 5	2.7	20	80465
6 - 7	4.6	20	80466
8 - 9	5.5	20	80467
10 - 11	7.3	20	80468
12 - 13	9.7	20	80525
14 - 15	11.9	20	80526





Water flow stopcocks, PE

With reinforced handles and strong tubing fittings.
Suitable only for non-pressurised operation.

For tubing with an inner Ø of Inches/mm	PU	Cat. No.
1/2" / 12	10	75093
3/8" / 9	10	75193



Non-return valve, PE-HD

With valve disc made from FKM. Max. operating pressure 2 bar.

For tubing with an inner Ø of mm	PU	Cat. No.
6 - 9	10	78593



Non-return valves, PP

With valve discs made from nitrile rubber (NBR). Max. operating pressure 2 bar.

For tubing with an inner Ø of mm	PU	Cat. No.
8 - 10	10	80418
10 - 15	10	80419

Lab assistants

PTFE-tape

For sealing and wrapping of threads and other connections. High chemical resistance.
Working temperatures up to 250 °C.

Length m	Width mm	PU	Cat. No.
12	12	10	131097





Trays, MF



White. Flat shape. Rounded corners. Smooth surfaces, easy to clean.
Practical tray for instruments, tools, and sensitive utensils. Stable and self-supporting.

L x W x H mm	PU	Cat. No.
190 x 150 x 17	5	71598
240 x 180 x 17	5	71698
268 x 208 x 17	5	71798
355 x 240 x 17	5	71898
428 x 288 x 17	5	71998



Trays, MF



White. Tall shape. Rounded corners. Smooth surfaces, easy to clean.
Practical tray for instruments, tools, and sensitive utensils. Stable and self-supporting.
Fitting lid made of PS, please order separately.

L x W x H mm	PU	Cat. No.
190 x 150 x 40	5	72098
290 x 160 x 35	5	72198
290 x 160 x 60	5	72398
340 x 245 x 100	5	72498
350 x 250 x 40	5	72298



Lids for trays, PS

Crystal clear. With handle. Rounded corners. Smooth surfaces, easy to clean.
Protects the contents of the instrument trays from dust and contamination.
The contents remain readily visible.

Size mm	For tray, MF No.	PU	Cat. No.
190 x 150	72098	5	79790
290 x 160	72198, 72398	5	79890
340 x 245	72498	5	79990*

* without handle

Lab assistants

Drawer organiser, PVC

White. With 9 lengthwise compartments opening at the front. For vials with a diameter of 25 mm.

Size mm	Height mm	PU	Cat. No.
355 x 300	45	1	80952



Drawer organiser, PVC

White. With 12 compartments. Ideal for the orderly storage of small components. Stabilising circumferential edge.

Size mm	Height mm	PU	Cat. No.
410 x 300	65	1	80953



Drawer organiser, PVC

White. Compartments of 5 different sizes for pipettes, thermometers, connectors, etc. Stabilising circumferential edge.

Size mm	Height mm	PU	Cat. No.
410 x 300	70	1	80954





Drying rack

Back plate and trough made from PVC with drainage nozzle.
 With 75 metal pegs (length: 10 cm) with PE coating for hanging various sizes of apparatus.
 With two bore holes for simple wall mounting.
 Delivered without installation hardware.

Size mm	PU	Cat. No.
450 x 630	1	76299



Drying rack, PS

With wide draining trough and drainage nozzles.
 Rack with 72 pegs 95 x 15 mm. For drying larger apparatus, some of the pegs can be removed and the bore holes closed at the rear.
 Delivered complete with drainage tube and accessories for the wall installation.
 In addition, 11 pegs (95 x 6 mm) are included for objects having a smaller diameter, such as reagent tubes.

Description	Size mm	PU	Cat. No.
Drying rack	450 x 630	1	80213
Pegs	95 x 6	11	81213

VITLAB[®] Promotional

ADVERTISE WITH YOUR GOOD NAME



VITLAB 
Competence in Labware

Your good name in daily use

Precision is usually of great significance when it comes to ensuring the effective use of granulates, powders or liquids. The transportation, storage and decanting of small volumes often require special containers. VITLAB is one of the leading manufacturers of high-grade plastic labware and specializes in high-precision printing on plastic products with superior chemical and break resistance.



This offers a great advantage: by having your name and logo printed on these products, you will work “hand in hand” with your clients and always maintain a high presence. The products can be used wherever people work with granulates, powders or liquids; for example, in agriculture, laboratories, the medical sector, the food industry and the cleaning

business, as well as when using colours and chemicals.

Plastic labware by VITLAB guarantees that you have the best manufacturing quality and optimal functionality associated with your good name, thus ensuring a sustained positive echo.



A positive echo through individuality

VITLAB develops and manufactures its products at its own production facilities. This allows us to produce and print plastic labware according to your individual requirements and specifications. Please do not hesitate to inform us of your wishes and we will let you know what sort of individual solution we can provide for you.

When it comes to precision and accuracy


Volumetric containers by VITLAB stand out due to the greater precision and accuracy ensured by the measuring scale. On request, VITLAB can also print a customized scale on your product. The quality colours guarantee that the scale remains readable and does not wear off.

Small gifts keep the friendship alive

Plastic products have a high level of usability and are ideally suited as advertising articles or for promotional campaigns for your products. You can have your company name and logo or other motifs printed on them permanently and thus advertise with your good name.

A unique position thanks to an unmistakable design

VITLAB provides advertising materials of the very highest quality with round, conical or flat printing, using screen or pad printing systems and with particularly durable and luminescent colours according to the Pantone and HKS colour table. Various marking techniques, such as laser printing and heat embossing, provide you with an unmistakable design.

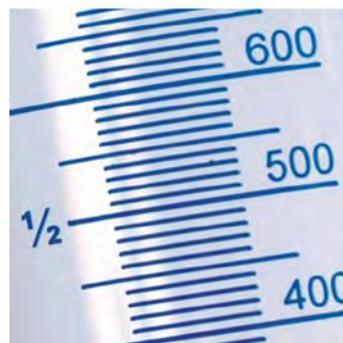

Would you like to have more information?

Please do not hesitate to contact us!

Please do not hesitate to contact us for advice on the selection, design and colour of your plastic products. A personal consultant ensures that you receive competent advice from the first meeting to the delivery of the product.

Our contact information:

Tel: +49 (0) 6026 977 99-0

Fax: +49 (0) 6026 977 99 -30

E-mail: info@vitlab.com

www.vitlab-promotional.com


Technical information

	Page
• Fluoroplastic PFA	130
• VITLAB [®] opaque	132
• Plastics and their properties	133
• Classification and type description of plastics	133
• Chemical stability of plastics	137
• Physical properties of plastics	146
• Cleaning and maintenance of plastics	147
• Sterilisation of laboratory equipment made of plastics	148
• Disposal and recycling	150
• Suitability for foodstuffs	150
• CE-IVD	151
• Accuracy of volumetric instruments	152


PFA evaporating dish



PTFE beaker

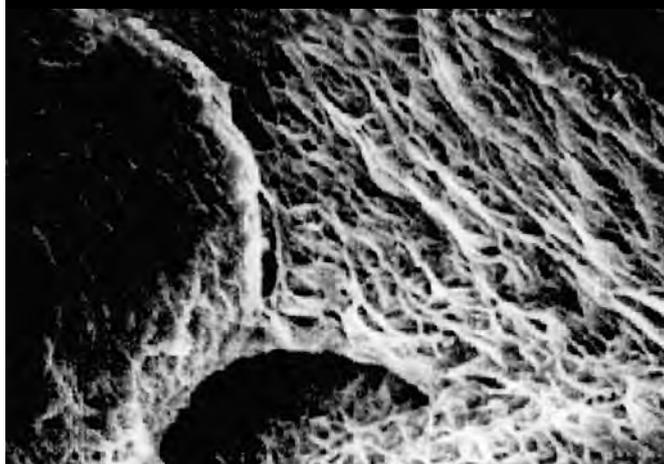

PE-HD bottle

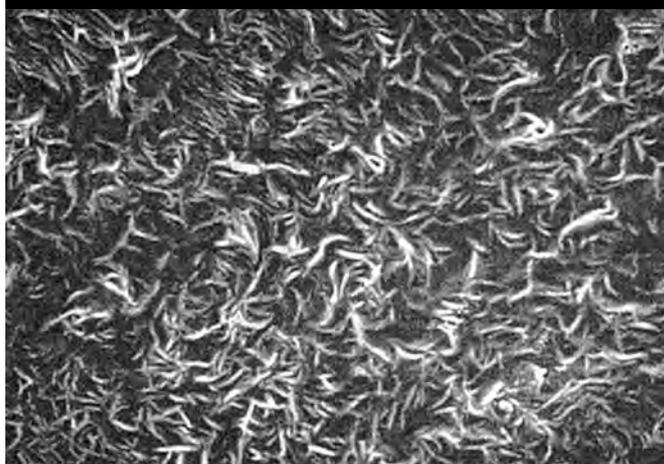

Fluoroplastic PFA

Today, trace analysis operates with concentrations in the range of ng/g (ppb) and pg/g (ppt). Thus, all modern processes require a corresponding trace analytical laboratory hygiene. However, the analytical accuracy of the measurement depends not only on the accuracy of the analytical instrument, but also directly on the judicious selection of container materials and the preparation of the samples themselves. Under these conditions, the fluoroplastic PFA truly shows its worth.

Labware made from polyolefins, such as polypropylene (PP) or polyethylene (PE), has found broad application in modern laboratories. Since catalysts (e.g., Ziegler-Natta or Philipps) are used during the manufacturing process, the constituent elements (frequently Al, Cr, Mg, Si, Ti or Zn) can still be detected in the ultra-trace range, and thus might affect the analysis results. In direct comparison to these manufacturing processes, PFA is especially suitable for trace element analysis because it is manufactured without the use of additives, and therefore cannot become contaminated by the additive components.

In addition to this advantage, PFA has other remarkable properties. PFA can be used for a broad range of applications by virtue of its resistance to almost all organic and inorganic compounds. PFA is one of the most resistant materials after platinum, and is practically chemically inert. Moreover, PFA stands apart with extraordinarily high thermal stability, making it possible to operate in the temperature range of -200 to +260 °C.

For all PFA products, VITLAB uses only high-purity PFA, which is particularly well-suited for trace analysis. For less critical uses, e.g. if the main requirement is a high chemical resistance, VITLAB offers bottles of "economy grade" PFA, which are partly made of recycled PFA. These are favourably priced and also environmentally friendly.


Pictures of the surface structure of PTFE, PFA, and PE-HD with a scanning electron microscope (8000 times magnification).

Technical information

VITLAB's PFA vessels have unique, extremely smooth, liquid-repellent surfaces that are made possible through modern manufacturing processes and acknowledged expertise (see pictures on "Surface Structure"). This is especially significant in the illustrative comparison. The pictures taken in a scanning electron microscope show uneven and irregular surfaces for PE-HD and PTFE, and deep pores and concavities can be identified in the PTFE surface. In contrast to the uneven surfaces, PFA evaporating dishes had to be marked (X) and exhibit a completely smooth, even and uniform surface structure.

Due to this characteristic, all PFA labware is particularly easy to clean and presents hardly any interactions with samples as compared to conventional container materials. With these advantages combined with the minimal water absorption by PFA (< 0.03%), even samples at very low concentration can be stored for long periods of time in PFA containers without changes in their concentration (see the application example on Mercury Standards).

Concentration 2 ppb (ng/g) each

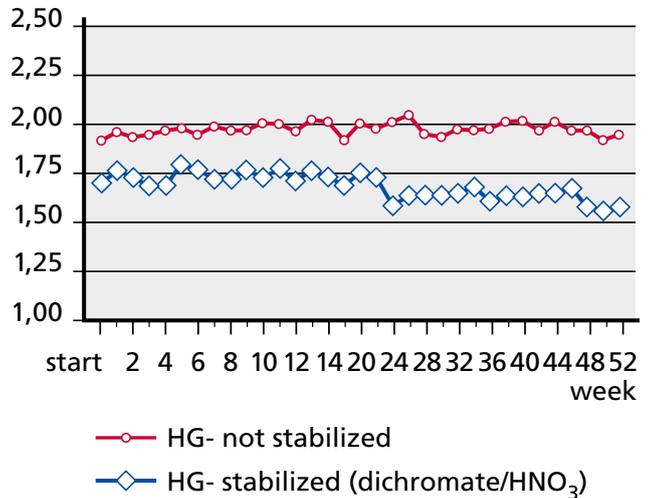


Application Example - Mercury Standards: Storage of an Hg standard in high-purity PFA containers (concentration 2 ppb (ng/g) each). Source: GIT Laboratory Trade Magazine 1/95

Cleaning after contamination

The valuable properties of PFA, primarily the near absence of memory effects, ensure the reliability of trace analytical results. In comparison with a commercially available glass flask, the simple cleaning after contamination with lead (Pb) solution at a concentration of 1000 ppb (ng/g) is a telling example (see the section on Cleaning of Volumetric Flasks). The cleaning of the glass and PFA volumetric flasks was conducted by shaking with 65% HNO₃ *Suprapur® (Pb < 0.005 ppm) at room temperature. With PFA volumetric flasks, the minimum concentration of 0.003 ppb is reached after three rinses, while substantially higher lead concentrations can be measured in glass flasks even after four rinses. The experiment also shows that PFA labware does not require the usual time-consuming boiling.

Mean of 4 Graduated Flask 500 ml each

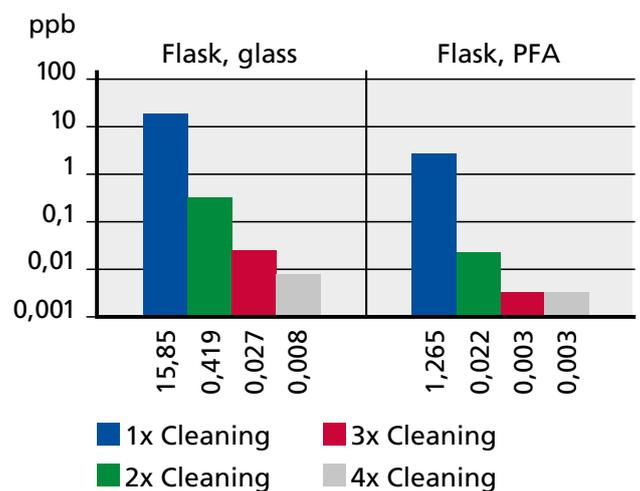

Cleaning of glass and PFA volumetric flasks after contamination. Source: Kali-Forschungsinstitut, K. Mangold

*Suprapur® is a trademark of Merck KGaA.

VITLAB® opaque



Greater protection for light-sensitive substances.

Light-sensitive substances require protection from the effects of light and particularly UV light so that they have a longer usable lifetime. In 2008, VITLAB manufactured the world's first opaque volumetric flasks developed from specially pigmented plastic. The special pigments safely protect samples from the effects of light, while still maintaining high transparency to enable volumes to be set accurately.

The opaque volumetric flasks and reagent bottles safeguard the contained substances with a light protection factor of virtually 20. The absorption spectrum properties exhibited by the products are significantly better over the entire spectral range of 200 - 900 nm versus comparable brown glass products. VITLAB® opaque reagent bottles are especially effective below 560 nm. They have a maximum of 5% transmission at 560 nm, and less than 2.5% transmission measurable at or below 520 nm. The pigments in the opaque products exhibit a brilliant characteristic shine in the UV range starting at 400 nm.

In the UV range from 280 nm and in the upper visible range from 580 nm, VITLAB® opaque reagent bottles and volumetric flasks are thus significantly better than even high-quality brown glass containers. The differences between reagent bottles made of VITLAB® opaque and those of brown glass bottles can be more or less pronounced depending on the type of the glass, since the brown glass bottles are subjected to significantly greater production fluctuations.

The higher break resistance and lower weight are advantageous during daily use in the laboratory, and make VITLAB® opaque an attractive alternative to conventional volumetric flasks and reagent bottles made of brown glass.

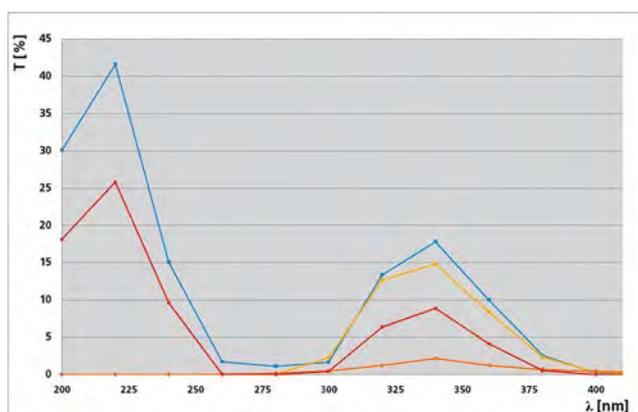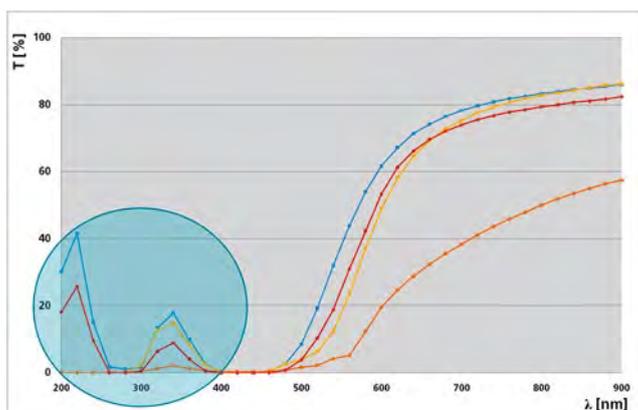

Light transmission diagram: Comparison of results for the measurement of transmission (T%) between VITLAB® opaque and brown glass in volumetric flasks and bottles, in the wavelength range of $\lambda = 200$ to 900 nm. VITLAB® opaque provides better protection of the container contents from the effects of light, particularly in the UV range (see diagram below).

- Brown glass volumetric flasks
- Brown glass bottle
- ◆— VITLAB® opaque bottle
- ◆— VITLAB® opaque volumetric flask



Classification and type description of plastics


In general, plastics can be divided into the three groups. The abbreviations of the described plastics used are those according to DIN 7728.

Thermoplastics

Plastics with a linear molecular structure, with or without side chains, can be reversibly moulded through heat treatment without changing their thermoplastic properties. Thermoplastics are frequently used in the production of plastic labware. Hence we provide here a brief description of some of the more important plastics, and explain their molecular structure, as well as their mechanical, chemical and physical properties. The most frequently used thermoplastics are polyolefins, such as polyethylene and polypropylene.


PFA (perfluoroalkoxy copolymer)

- 121°C
- Highly transparent, elastic thermoplastic with high-molecular, semi-crystalline structure
- Very good temperature stability
- Broad range of application, from -200 °C to +260 °C
- Virtually chemically inert, excellent chemical stability against practically all chemicals
- Very low water absorption (< 0.03%)
- Ultra-smooth, anti-adhesive surface with unique surface structure
- Typical products are, for example: Class A volumetric flasks, bottles, sample containers
 - ➔ Especially suitable for use in trace analysis, and for the storage of low-concentration solutions




PTFE Polytetrafluoroethylene

- 121°C
- Non-transparent, white, elastic thermoplastic with high-molecular, semi-crystalline structure
- Very good temperature stability
- Broad range of application, from -200 °C to +260 °C
- Virtually chemically inert, excellent chemical stability against practically all chemicals
- Anti-adhesive surface
- Very good sliding properties and electrical insulating capability (very low friction coefficient)
- Typical products are, for example: Bottles, beakers, sheathing for magnetic stir bars




FEP Tetrafluoroethylene-perfluoropropylene copolymer

- 121°C
- Translucent, white, thermoplastic copolymer with high-molecular, semi-crystalline structure
- Anti-adhesive surface
- Very good temperature stability
- Broad range of application, from -100 °C to +205 °C
- Excellent chemical stability




ETFE Ethylene-tetrafluoroethylene copolymer

- 121°C
- Translucent, white copolymer from ethylene and tetrafluoroethylene
- Very good temperature stability
- Broad range of application, from -100 °C to +150 °C
- Very good chemical stability
- Typical products are, for example: Thread adapters, Griffin beakers, threaded connectors




PMP Polymethylpentene

- 121°C
- Crystal-clear, stiff thermoplastic
- Similar structure to PP, with the methyl group replaced by an isobutyl group
- Good thermal stability
- Range of application from 0 to +150 °C
- Good tensile strength and dimensional stability
- Good chemical stability
- Typical products are, for example: Class A volumetric flasks, Class A measuring cylinders
 - ➔ For the storage of light-sensitive substances, also available in highly transparent, UV-absorbing VITLAB® opaque




Classification and type description of plastics



PP Polypropylene


121°C

- Highly transparent, elastic thermoplastic
- Similar structure to PE, with a methyl group attached to alternate carbon atoms in an isotactic arrangement
- Good thermal stability
- Range of application from 0 °C to +125 °C
- Good tensile strength and dimensional stability
- Good chemical stability, comparable to PE
- Typical products are, for example: Class B volumetric flasks, Class B measuring cylinders, measuring pitchers, sample containers, funnels
 - ➔ For the storage of light-sensitive substances, also available in highly transparent, UV-absorbing VITLAB® opaque




PE-HD High-density polyethylene

- Transparent, elastic thermoplastic
- Good thermal stability
- Range of application from -50 °C to +105 °C
- Compact, with increased tensile strength due to less cross-linking compared with PE-LD
- Good chemical stability
- Better chemical stability to organic solvents compared to PE-LD
- Typical products are, for example: Bottles, buckets, scoops
 - ➔ For the storage of light-sensitive materials, also available in brown-dyed version



PE-LD Low-density polyethylene


- Highly transparent, elastic thermoplastic
- Moderate thermal stability
- Range of application from -50 °C to +80 °C
- Very good flexibility
- Good chemical stability
- Typical products are, for example: Wash bottles, dropping pipettes



PC Polycarbonate

121°C

- Transparent, stiff thermoplastic
- Linear polymer of carbon dioxide
- Very good temperature stability
- Broad range of application, from -130 °C to +125 °C
- Good tensile strength and impact resistance
- Moderate chemical stability
- Typical products are, for example: Desiccators
- Note: Polycarbonates can lose their tensile strength through autoclaving or exposure to alkaline detergents



POM Polyoxymethylene


121°C

- Non-transparent, white, stiff, and high-molecular thermoplastic
- Good thermal stability
- Broad range of application, from -40 °C to +130 °C
- High hardness and dimensional stability
- Good sliding properties and abrasion resistance
- Good chemical resistance to aliphatic, aromatic, and halogenated hydrocarbons, and alkalis. Unstable to acids and esters
- Typical products are, for example: Slide boxes, staining jars
 - ➔ Especially good chemical stability to organic solvents
 - ➔ POM can replace metal in many applications

Classification and type description of plastics


PA Polyamide

- Linear polymers with regularly repeating amide bonds along the main chain
- Good thermal stability
- Range of application from -40 °C to +100 °C
- Outstanding durability and tensile strength, often used as construction material and for metal coatings
- Good chemical resistance to organic solvents
- Readily attacked by acids and oxidising agents
- Typical products are, for example: Spatula




SAN Styrene-acrylonitrile copolymer

- Crystal clear, stiff thermoplastic copolymer
- Moderate thermal stability
- Range of application from -40 °C to +70 °C
- Brittle and dimensionally stable
- Low tendency to form stress cracks
- Moderate chemical stability, SAN is slightly more chemically stable than PS
- Typical products are, for example: Graduated beakers, Class B graduated cylinders




PMMA Poly(methyl methacrylate)

- Crystal clear ("organic glass"), dimensionally stable thermoplastic
- Moderate thermal stability
- Range of application from -50 °C to +65 °C
- Very good UV radiation stability
- Poor chemical stability
- Typical products are, for example: Cuvettes




PS Polystyrene

- Crystal clear, stiff, amorphous or semi-crystalline thermoplastic
- Moderate thermal stability
- Range of application from -20 °C to +70 °C
- Hard, brittle, and dimensionally stable
- Tendency to form stress cracks
- Moderate chemical stability
- Typical products are, for example: Containers, cuvettes



PVC Poly(vinyl chloride)


- Amorphous thermoplastic, transparent with a slight blue tint
- Moderate thermal stability
- Range of application from -20 °C to +80 °C
- Good chemical stability, especially resistant to oils
- The addition of plasticisers opens up many useful applications, ranging from artificial leather to injection moulding components
- Typical products are, for example: Drawer organisers, dishes, trays



Classification and type description of plastics

Thermosets

Plastics with densely cross-linked molecules, which are very hard and brittle at normal temperatures. Heating causes irreversible hardening. These plastics are rarely used for plastic labware. The best known thermosets are the melamine resins. Melamine resin is produced by polycondensation of melamine with formaldehyde.




MF Melamine-formaldehyde resin

- Colourless thermoset, also belongs to the aminoplast group
- Good thermal stability
- Broad range of application, from -80 °C to +120 °C
- High surface hardness, abrasion resistance, and fire resistance
- Good electrical insulator, high creep resistance
- Good chemical stability
- Typical products are, for example: Trays, plates, mixing bowls
- Caution necessary when used in a microwave oven: Heating can release amounts of melamine and formaldehyde that can be harmful to health!


Elastomers

Plastics with loosely cross-linked molecules that exhibit rubber-like elasticity at room temperature. Heating causes irreversible integration (vulcanisation). The best known elastomers are natural rubber and silicone rubber.




NR Natural rubber

- Elastomer obtained from latex (milk-like sap from rubber tree bark) and vulcanised with sulphur to improve the elasticity
- Composed of polymerised isoprene, with an extremely uniform structure
- Moderate thermal stability, not stable to UV
- Range of application from -40 °C to +80°C
- High tensile strength and elongation at rupture
- Poor chemical stability
- Typical products are, for example: pipette filler bulbs



SI Silicone rubber

- Synthetic elastomer in which silicon atoms are linked together by oxygen atoms
- Includes polyorganosilanes that have groups such as hydrogen atoms, hydroxyl groups or vinyl groups for cross-linking reactions
- Very good thermal stability, and resistance to UV, ozone, and weather
- Broad range of application, from -60 °C to +180 °C
- High dimensional stability, even at high temperatures
- Very good durability, even at low temperatures
- Poor chemical stability



EPDM Ethylene-propylene-diene rubber

- Synthetic terpolymeric elastomer
- Manufactured with metallocene or Ziegler-Natta catalysts that utilise vanadium compounds and aluminium alkyl chlorides
- Good thermal stability
- Range of application from -40 °C to +130 °C
- High elasticity, even at low temperatures
- Stable to UV and ozone, and weather-resistant
- Very good chemical stability

Technical information

Chemical resistance of plastics

With regard to chemical stability, plastics are classified as follows:

<p style="font-size: 2em; font-weight: bold;">+</p> <p style="font-weight: bold;">Very good chemical resistance</p> <p>Within 30 days, continuous exposure to media causes no damage to the plastic. The plastic may remain resistant for years.</p>	<p style="font-size: 2em; font-weight: bold;">0</p> <p style="font-weight: bold;">Good to limited chemical resistance</p> <p>Within 7-30 days, continuous exposure to media causes minor damage (e.g. swelling, softening, loss of mechanical strength, discolouration), some of which is reversible.</p>	<p style="font-size: 2em; font-weight: bold;">-</p> <p style="font-weight: bold;">Poor chemical resistance</p> <p>Not suitable for continuous exposure to media. Immediate damage may occur (e.g. loss of mechanical strength, deformation, discolouration, cracking, liquification).</p>
--	---	---

Chemical resistance of plastics to various substance classes

Classes of substances at 20 °C	PFA	PTFE	FEP	ETFE	PMP	PP	PE-HD	PE-LD	PC	POM	PA	SAN	PMMA	PS	PVC	MF	NR	SI	EPDM	FKM
Alcohols, aliphatics	+	+	+	+	+	+	+	+	+	+	0	+	-	+	+	+	+	+	+	-
Ethers	+	+	+	+	-	0	0	0	-	+	+	-	-	-	-	-	-	-	-	-
Aldehydes	+	+	+	+	0	+	+	0	0	0	0	-	0	-	-	+	0	0	+	+
Esters	+	+	+	+	0	0	0	0	-	-	+	-	0	-	-	+	0	0	0	-
Hydrocarbons, aliphatic	+	+	+	+	0	+	+	0	0	+	0	-	+	-	+	+	-	-	-	0
Hydrocarbons, aromatic	+	+	+	+	-	0	+	0	-	+	0	-	-	-	-	+	-	-	-	0
Hydrocarbons, halogenated	+	+	+	+	-	0	0	0	-	+	0	-	-	-	-	+	-	-	-	0
Ketones	+	+	+	0	0	0	0	0	-	+	+	-	-	-	-	+	-	-	0	-
Alkalis	+	+	+	+	+	+	+	+	-	+	+	+	+	+	+	-	+	0	+	0
Acids, strong or concentrated	+	+	+	+	+	+	+	+	-	-	-	-	-	0	+	-	-	-	+	0
Acids, weak or diluted	+	+	+	+	+	+	+	+	0	-	-	0	-	0	+	0	0	0	+	+
Oxidising acids, oxidising agents	+	+	+	+	-	-	-	-	-	-	-	-	-	-	-	-	-	-	0	0

The carefully prepared recommendations listed here are based on technical literature and made available by the manufacturers of raw materials, to provide information and advice. However, nothing can replace suitability tests conducted by the end user under the actual conditions of use.

Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Acetaldehyde	+	+	+	+	+	0	0	-	+	-	+	0	+	-
Acetic acid (glacial acetic acid), 100%	+	+	+	+	+	+	+	0	+	0	+	+	+	0
Acetic acid, 50%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Acetic anhydride	+	+	+	+	+	+	+	0	0	0	0	0	-	-
Acetone	+	+	+	+	+	0	+	+	+	+	+	+	+	0
Acetonitrile	+	+	+	+	+	+	0	-	+	0	+	0	+	0
Acetophenone	+	+	+	+	+	+	0	-	0	0	0	0	-	-
Acetyl chloride(acetic acid chloride)	+	+	+	+	+	+			+		+		+	
Acetylacetone	+	+	+	+	+	+	+		+		+		+	
Acrylic acid (2-propenic acid)	+	+	+	+	+	+	+		+		+		+	
Acrylonitrile	+	+	+	+	+	+	-	-	0	-	+	+	+	+
Adipic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Allyl alcohol (2-propan-1-ol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Aluminium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Aluminium hydroxide	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Amino acids	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium fluoride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium hydroxide, 30% (ammonia)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium sulphate			+	+			+	+	+	+	+	+	+	+
n-Amyl acetate (pentyl acetate)	+	+	+	+	+	+	+	0	0	-	+	0	0	-
Amyl alcohol (pentanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Amyl chloride (chloropentane)	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Aniline	+	+	+	+	+	0	+	0	+	+	+	+	+	0
Aqua regia	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Barium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Benzaldehyde	+	0	+	+	+	0	+	+	+	+	+	+	+	+
Benzene	+	+	+	+	+	+	0	0	+	0	+	+	0	-
Benzoyl chloride			+	+	+	+	0	0	+	0	+	+	0	-
Benzyl alcohol	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Benzyl chloride			+	+	+	+								
Benzylamine	+	+	+	+	+	+	0		0		0		0	-
Boric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Bromine	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Bromobenzene	+	+	+	+	0	-	-	-	-	-	-	-	-	-
Bromoform	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Bromonaphthalene	+	+	+	+	+	+								
Butanediol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
1-Butanol (butyl alcohol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
n-Butyl acetate (acetic acid n-butyl ester)	+	+	+	+	+	+	+	0	0	0	+	+	0	0
Butyl methyl ether	+	+	+	+	+	0	+	-	+	0	0	-	0	-
Butylamine			+	+	+	+								
Butyric acid (butanoic acid)	+	+	+	+	+	+			-	-	0	-	-	-
Calcium carbonate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium hypochlorite	+	+	+	+	+	+	+	0	+	+	+	+	+	+

Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C																
0	-	+	+	0		-	-	-	-	-	-	-	-		-	-	0	-
-	-	-	-	-	-					-	-			0	0	0	0	-
+	0	0	-	-	-	+	0	-	-	0	0	+	0	+	-	-	-	-
-	-	-	-	0	0					-	-	-	-		0	0	0	-
-	-	+	+	+		-	-	-	-	-	-	-	-	+	0	-	+	-
-	-	+		+		-	-	-	-	-	-	-	-		-	-	-	-
-	-	+		+		-	-	-	-	-	-	-	-	+	-	-	+	-
-	-			-	-	-	-	-	-	-	-	-	-		-	-	-	+
-	-	+				-	-	-	-	-	-	-	-		-	-	+	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	-
+	+	+	+	+		+	+	+	+	+	+	+	0		+	+	+	+
0	0	+	+	0		0	-	-	-	0	0	0	-		0	-	+	+
-	-	+	0	0	-	+	+	+	+	+	+	+	0	+	0	0	+	+
0	-	+	+	+	+	0	0	0	0	0	0	+	+		+	+	+	+
+	+	+	+	+	+	+	+	+	+	+	+	+	+		+	+	+	+
0	0	+	+	+		+	+	0	0	+	+	+	0		+	+	+	+
0	0	+	+	+		+	+	0	0	+	+	+	0		-	+	+	0
-	-	0	0	0		+	0	+	+	0	-	+	0	+	+	0	+	-
+	+	+	+	+		+	+	+	+	+	+	+	+		0	0	+	-
-	-	+	+	0		-	-	+	+	-	-	-	-		0	-	0	-
+	+	+	+	+		+	+			0	0	0	0		0	-	0	0
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	+
0	-	0	0	0	-	-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
0	-	+	+	0		-	-	-	-	-	-	-	-		-	-	0	-
-	-	+	0	+		-	-	-	-	-	-	-	-	+	-	-	-	0
-	-	+	0	-	-	-	-	-	-	-	-	-	-		-	-	-	+
0	0	+	+	-	-	-	-	-	-	-	-	0	0		-	0	0	+
		+		+		-	-	-	-	-	-				-	-	-	+
-	-	+				-	-	-	-	-	-	-	-		-	0	0	+
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	0
-	-			+		-	-	-	-	-	-	-	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-		
		+	+	+		-	-	-	-	-	-				0	-	+	-
0	0	+	+	+	0	+	0	0	-	0	-	0	0		+	0	0	+
-	-	+	0	+		-	-	-	-	-	-	-	-		-	-	0	-
-	-	+	+			-	-	-	-	-	-	-	-		-	-	-	-
		+	+			-	-			-	-				-	0	-	-
0	-			0	0	-	-			-	-				-	-	-	0
+	+	+	+	+	+	+	+	+	+	+	+	+	+		+	+	+	+
+	+	+	+	-	-	+	+	+	+	+	+	0	-		+	+	+	+
-	-	+	+	+		+	0	+	+	+	0	+	+		+	0	+	+
0	-	+	+	+	-	+	+	0	0	+	+	0	-		-	0	+	+

Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Carbon disulphide	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Carbon tetrachloride	+	+	+	+	+	+	-	-	-	-	0	-	0	-
Chloroacetaldehyde, 45%			+	+	+	+								
Chloroacetic acid (monochloroacetic acid)	+	+	+	+	+	+	+	0	+	0	+	+	+	+
Chloroacetone			+	+	+	+								
Chlorobenzene	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Chlorobutane	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Chloroform	+	0	+	+	+	0	0	-	-	-	0	-	0	-
Chloronaphthalene			+	+	+	+								
Chlorosulphonic acid	+	+	+	+	0	-								
Chromic acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Chromic acid, 50%	+	+	+	+	+	+	0	0	0	0	+	0	+	0
Chromic-sulphuric acid	+	+	+	+	+	+	0	-	-	-	-	-	-	-
Copper sulphate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Cresol	+	+	+	+	+	0	-	-	0	0	0	-	-	-
Cumene (isopropylbenzene)	+	+	+	+	+	+	-	-	0	-	+	0	0	-
Cyclohexane	+	+	+	+	+	0	-	-	0	-	0	-	0	-
Cyclohexanone	+	+	+	+	+	+	0	0	0	-	0	-	-	-
Cyclopentane	+	+	+	+	+	+	0	-	0	-	0	-	-	-
Decane	+	+	+	+	+	+	0		0		0	-		
1-Decanol	+	+	+	+	+	+	+		+		+			
Di(ethylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Dibenzyl ether	+	+	+	+	+	+	0		+		+			
Dibromoethane	+		+	+	0									
Dibutyl phthalate	+	+	+	+	+	+	+	0	+	0	0	-	0	-
Dichloroacetic acid	+	+	+	+	+	0	+	+	0	-	0	0	0	-
Dichlorobenzene	+	+	+	+	+	0	-	-	0	-	0	-	0	-
Dichloroethane	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Dichloromethane (methylene chloride)	+	+	+	+	0	0	0	-	0	-	0	-	0	-
Diesel oil (heating oil)	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Diethanolamine			+	+					0		0			
Diethyl ether	+	+	+	+	+	+	-	-	0	-	0	-	-	-
Diethylamine	+	+	+	+	+	0	0	0	0	-	0	-	-	-
1,2 Diethylbenzene	+	+	+	+	+	0	-	-	-	-	0	-	-	-
Dimethyl sulphoxide (DMSO)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Dimethylaniline	+	+	+	+	+	+								
Dimethylformamide (DMF)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
1,4-Dioxane	+	+	+	+	+	0	0	0	+	0	+	+	+	0
Diphenyl ether			+	+										
1,2 Ethanediol (ethylene glycol, glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ethanol (ethyl alcohol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Ethanolamine	+	+	+	+	+	+			+					
Ethyl acetate (acetic acid ethyl ester)	+	+	+	+	+	+	0	-	+	0	+	+	+	+
Ethyl methyl ketone (MEK)	+	+	+	+	0	0	-	-	+	0	0	-	0	-
Ethylbenzene	+	+	+	+	0	0	-	-	-	-	-	-	-	-
Ethylene oxide	+	+	+	+	+	+	0	-	0	-	0	0	0	0
Fluoroacetic acid			+											

Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C																
-	-	+	+	0		-	-	-	-	-	-	-	-		-	-	-	+
-	-	0	0	-	-	-	-	0	-	-	-	-	-	+	-	-	-	+
0	-	-	-	-	-	-	-	0	-	0	-	+	0		-	-	0	0
															0	-	+	-
-	-			-	-	-	-	-	-	-	-	-	-		-	-	-	0
		-	-															0
-	-	-	-	0	-	-	-	-	-	-	-	-	-	+	-	-	-	0
		-	-												-	-	-	+
		-	-	-	-										-	-	-	-
+	0	0	0	-	-	-	-	0	-	-	-	+	0		-	0	-	+
0	-	-	-	-	-	0	0	-	-	-	-	+	-		-	-	-	+
-	-	-	-	-	-	0	0	-	-	0	0	+	0		-	-	-	+
+	+	+	+	+		+	0	+	+	+	+	+	0		0	+	+	+
-	-			-	-					-	-	-	-		-	-	-	+
-	-	+	-			-	-	-	-	-	-	-	-		-	-	-	+
-	-	+	+	+						-	-	-	-	+	-	-	-	+
-	-			+						-	-	-	-		-	-	-	-
-	-									-	-	-	-		-	-	-	+
0		+				0				0		+			0	0	-	+
0		+				0				0		+			0	0	+	+
0	0	+	0	0		+	+	-	-	0	-	-	-		+	0	+	+
		+				-	-	-	-	-	-				-	-	0	-
-	-	+	+			-	-	-	-	-	-	-	-		-	0	0	0
0	-			-	-					0	-	0	-		-	-	-	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	+
		-	-	0											-	-	-	0
-	-			0	-					-	-	-	-		-	-	-	0
-	-	+	+	+	+	-	-	0	-	-	-	0	-		-	-	-	+
-	-					-	-	-	-	-	-						0	
-	-	+	+	+	+	-	-	-	-	-	-	-	-		0	0	0	-
0	0	0	0	+		-	-	-	-	-	-	-	-		-	-	0	-
		0		0		-	-	-	-	-	-				-	-	-	0
+	+	+	+	0	0	+	+	+	+	+	+	+	+	+	-	+	+	0
+	0	+	+	+		0	-	-	-	0	-	+	0	+	0	0	+	0
															-	-	+	
-	-			+		-	-			-	-	-	-	+	-	-	0	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	-
-	-					-	-	-	-	-	-	-	-		-	-	-	0
0	-	+	+	0		-	-	-	-	-	-	0	-		-	-	-	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	-	-

Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Formaldehyde, 40%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Formamide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Formic acid, 98-100%	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Gasoline (petroleum spirits)	+	+	+	+	+	+	0	0	0	0	+	+	0	-
Glycerine	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Glycolic acid, 70%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Heating oil (Diesel oil)	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Heptane	+	+	+	+	+	+	0	0	0	0	0	0	0	-
Hexane	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Hexanoic acid			+	+										
Hexanol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 20%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 37%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrofluoric acid, 40%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrofluoric acid, 70%	+	+	+	0	+	+	+	0	+	0	+	0	+	-
Hydrogen bromide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrogen peroxide, 35%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydroiodic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isoamyl alcohol (3-methyl-1-butanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isobutanol (isobutyl alcohol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isooctane	+	+	+	+	+	+								
Isopropanol (2-propanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isopropyl ether	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Lactic acid (2-hydroxypropionic acid)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Lugol's solution (iodine/potassium iodide solution)	+	+	+	+	+	+	+	0	+	+	-	-	-	-
Mercury	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Mercury chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Methanol	+	+	+	+	+	+	+	+	+	+	+	+	+	0
Methoxybenzene	+	+	+	+	+	+								
Methyl butyl ether	+	+	+	+	+	0	+	0	+	+	0	-	-	-
Methyl ethyl ketone (MEK)	+	+	+	+	0	0	-	-	+	0	0	-	0	-
Methyl formate (formic acid methyl ester)	+	+	+	+	+	+								
Methyl propyl ketone	+	+	+	+	+	+	0	0	+	0	+	+	+	0
Methylene chloride (dichloromethane)	+	+	+	+	+	+	-	-	0	-	0	-	0	-
Mineral oil (motor oil)	+	+	+	+	+	+	+	+	+	+	+	+	+	0
Monochloroacetic acid	+	+	+	+	+	+	+	0	+	0	+	+	+	+
Nitric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Nitric acid, 30%	+	+	+	+	+	+	0	-	0	-	0	-	0	0
Nitric acid, 70%	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Nitrobenzene	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Oleic acid	+	+	+	+	+	+								
Oxalic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ozone	+	+	+	+	+	+	+	+	0	-	0	-	0	-
n-Pentane	+	+	+	+	+	+								
Peracetic acid	+	+	+	+	+	+								
Perchloric acid	+	0	+	+	+	+	0	-	+	-	+	-	+	-
Perchloroethylene	+	+	+	+	+	+	-	-	-	-	-	-	-	-

Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C																
+	0	+	+	+	0	+	+	-	-	-	-	0	-		0	0	+	0
		-	-	+											+		0	0
+	0	-	-	-	-	0	0	-	-	+	0	-	-	+	0	-	0	-
0	-	+	+	+		-	-	+		-	-	0	-	+	-	-	-	+
+	+	0	0	+	+	+	+	+	+	+	+	+	+	+	0	+	+	0
				-	-										+	+	+	0
-	-	+	+	+		-	-	0	-	-	-	0	-		-	-	-	+
+	0			+				0	-	-	-	-	-		-	-	-	+
-	-	+	+	+		+	+	0	0	-	-	0	-		-	-	-	+
								+										
								+							0	0	-	+
-	-	-	-	-	-	0	-	0	-	+	+	+		-	0	0	+	+
0	0	-	-	-	-	0	-	0	-	+	+	0		-	0	-	+	+
-	-	-	-	-	-	0	-	0	-	0	0	0	-	-	0	-	+	0
-	-	-	-	-	-	+	0	-	-	+	+	0	-	-	-	-	0	0
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
+	+	-	-	-	-					0	-				0	-	0	+
+	+	+	-	-	-	+	+	-	-	+	+	+	0	0	-	0	0	
																	+	+
		+	+												0	0	0	0
+	+	+	+			0	-	0	-	0	0	+	0		+	+	+	+
0				+		0	-			0	-				-	-	-	+
+	+	+	+	+		+	-	0	-	0	0	+	0		+	0	+	+
-	-			-	-					-	-	-	-		-	-	-	-
+	+	+	-	0	-	+	+	0	-	+	+	0	0		0	0	0	+
0	-	0	0			0	-	-	-	0	-	-	-		+	-	+	+
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
+	+	0	0	-	-	+	+	+	+	+	0	-	-		+	+	+	+
+	0	+	+	0		0	-	-	-	0	-	+	0		0	+	+	-
-	-	0				-	-	-	-	-	-				-	-	-	-
-	-	0				-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	0	-
-	-	+				-	-	-	-	-	-	-	-		-	0	0	
-	-	+	+			-	-	-	-	-	-	-	-		-	-	0	-
-	-	-	-	0	-	-	-	-	-	-	-	-	-		-	-	-	0
+		+	+			+		+	+	+		+	+		-	0	-	+
0	-	-	-	-	-	-	-	0	-	0	-	+	0		-	-		0
+	0	-	-	-	-	+	0	+	0	-	-	+	0	-	-	-	0	0
+	0	-	-	-	-	0	-	0	0	-	-	0	-	-	-	-	-	0
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	-
-	-	0	-	-	-	-	-	-	-	-	-	-	-		-	-	-	-
				+		-	-	-	-	-	-				-	-	-	0
+	+	+	+	-	-	+	+	+	+	+	+	+	+		0	0	+	+
-	-	-	-	-	-	0	0	+	0	0	0	+	0		-	+	+	+
				+											-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	0	-		-	-	0	+
-	-	+	0	-	-	0	0	0	-	-	-	-	-		-	-	-	0

Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Petroleum	+	+	+	+	+	+	0	0	0	-	0	-	0	-
Petroleum ether	+	+	+	+	+	+							0	
Phenol	+	+	+	+	+	+	0	0	+	+	+	+	+	0
Phenylethanol	+	+	+	+	+	+			0		0			
Phenylhydrazine	+	+	+	+	+	+			0		0			
Phosphoric acid, 85%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Piperidine	+	+	+	+	+	+			+		+			
Potassium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Potassium dichromate			+	+										
Potassium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Potassium permanganate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Propanol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Propionic acid	+	+	+	+	+	0	+	0	+	0	+	0	0	-
Propylene glycol (propanediol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Pyridine	+	+	+	+	-	-	+	0	0	0	+	0	+	0
Salicylaldehyde	+	+	+	+	+	-	+	+	+	+	+	+	+	+
Salicylic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Silver acetate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Silver nitrate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium acetate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium dichromate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium fluoride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sulphuric acid, 60%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sulphuric acid, 98%	+	+	+	+	+	+	+	+	-	-	0	-	0	-
Tartaric acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Tetrachloroethylene	+		+	+	0									
Tetrahydrofuran (THF)	0	0	+	+	+	0	0	-	-	-	0	-	0	-
Tetramethylammonium hydroxide	+	+	+	+	+	+								
Toluene	+	+	+	+	+	+	0	-	0	-	0	0	0	-
Tri(ethylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Tri(propylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Trichloroacetic acid	+	+	+	+	+	0	+	+	0	-	0	0	0	-
Trichlorobenzene	+	+	+	+	+	0	0	0	-	-	-	-	-	-
Trichloroethane	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Trichloroethylene	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Trichlorotrifluoroethane	+	+	+	+	0	-								
Triethanolamine	+	+	+	+										
Trifluoroacetic acid (TFA)	+	-	+	0										
Trifluoroethane	+	0	+	+										
Turpentine	+	+	+	+	+	+	0	0	-	-	0	-	0	-
Urea	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Xylene	+	+	+	+	+	+	0	-	-	-	0	-	0	-
Zinc chloride, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Zinc sulphate, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+

Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C																
0	0	+	+	+				+		-	-	+	-		-	0	-	+
		+	+	+				+		-	-	0	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	0
				0											0	-	-	0
+	+	+	-	-	-	+	+	-	-	+	0	+	0	-	-	-	0	+
															-	-	-	-
+	+	+	+	+		0	0	+	+	0	0	+	0		+	+	+	+
				-	-										0	0	+	0
-	-	+	+	+		0	0	+	+	0	0	0	0	-	0	-	+	-
+	+	0	0	-	-	+	0	+	+	+	+	+	+		-	-	+	+
0		+	+	+	+	+	+	0		0		+	+		+	0	+	+
-	-	-	-	0	0					0	-	0	-		-	-	0	+
+	0	+	+	-	-	-	-	0	0	+	+	0	-		+	+	+	+
-	-	+	0	+		-	-	-	-	-	-	0	-		-	-	-	-
0	0					-	-			-	-	-	-					
		-	-	+		+	+			+	+	0	-		+	+	+	+
+	+	0	0			0	0	0	0	0	0	0	0		+	+	+	+
+	+	0	0	+		+	+	+	+	0	0	0	0		+	+	+	+
+	+	+	0	+		+	+	-	-	+	+	0	0		+	0	+	-
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
+	-	+	+	+		+	0	+	0	+	0	+	+		+	0	+	+
+	+	+	+	+		+	+	+	+	+	+	+	+		0	0	+	+
-	-	+	+	+	0	+	+			+	+	+	+	-	0	0	+	0
0	0	-	-	-	-	+	0	-	-	-	-	0	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	+
+	+	+	+	0	0	+	+	0	0	+	+	+	+	-	+	+	0	+
				-	-										-	-	-	0
-	-	0	0	+		-	-	-	-	-	-	-	-	+	-	-	-	-
-	-	-	-														+	-
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	0
+	0	+	0			+	+	0	0	+	+	0	-		0	+	+	+
+	0	+	0			+	+	0	0	+	+	0	-		+	+		
0	-			-	-					0	-	0	-		0		0	-
-	-									-	-	-	-					
-	-	0	-	0		-	-	-	-	-	-	-	-		-	-	-	+
-	-	-	-	0		-	-	-	-	-	-	-	-		-	-	-	0
				0		-	-			-	-						0	
						-	-			-	-				0	-	0	-
		-	-			-	-			-	-							-
						-	-			-	-				-	-	-	+
-	-	+	+	+		0	0	+	+	-	-	+	+		-	-	-	+
-	-	+	+	+		+	+	+	+	+	+	0	-	+	+	+	+	+
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	0
+	+	+	0	-	-	+	+	-	-	+	+	+	0		+	+	+	+
+	+	0	-	-	-	+	+	0	0	+	+	+	0		0	+	+	+

Physical properties of plastics

Plastics	Max. temperature for use °C	Brittleness temperature °C	Microwaveability*	Density g/cm ³
PFA	260	-200	yes	2,17
PTFE	260	-200	yes	2,17
FEP	205	-100	yes	2,15
ETFE	150	-100	yes	1,70
PMP	150	0	yes	0,83
PP	125	0	yes	0,90
PE-HD	105	-50	yes	0,95
PE-LD	80	-50	yes	0,92
PC	125	-130	yes	1,20
POM	130	-40	no	1,42
PA	90	0	-	1,13
SAN	70	-40	no	1,03
PMMA	65 - 95	-50	no	1,18
PS	70	-20	no	1,05
PVC	80	-20	no	1,35
MF	120	-80	yes**	1,50
NR	80	-40	no	1,20
SI	180	-60	no	1,10
EPDM	130	-40	-	-
FKM	220	-30	-	-

* Mind the chemical and temperature suitability!

** Caution necessary when used in a microwave oven: Heating can release amounts of melamine and formaldehyde that can be harmful to health!

Cleaning and maintenance of plastics

All polyolefins, such as PE-LD, PE-HD, PP and PMP, as well as the fluoroplastics PTFE, PFA, FEP and ETFE have water-repellent surfaces that are very durable and easy to clean. For cleaning, depending on the level of contamination, commercially available neutral or alkaline detergents can be used. Polycarbonate (PC) labware should not be cleaned with alkaline cleaning agents (> pH 7). Please note that no scrubbing agents or scouring pads should be used for labware made from plastics.

Cleaning with dishwashers

Labware made from the above-named plastics (except for PE-LD, due to the temperature limit) can be cleaned and dried in a laboratory dishwasher together with other apparatus. Machine cleaning with laboratory dishwashers is gentler to labware than cleaning in an immersion bath. The labware is exposed to the cleaning solution for relatively short rinsing periods when sprayed by the jet or injector nozzles. Due to their light weight, we recommend securing the apparatus to be washed with washing nets to prevent them from tumbling in the water jet. Labware is better protected against scratching when the wire baskets in the washing machine are plastic coated.

Cleaning in an ultrasonic bath

Plastic labware may be cleaned in an ultrasonic bath. However, direct contact with the acoustic membrane should be avoided.

Cleaning in trace analysis

To avoid contamination with cations and anions in trace analysis, plastic labware should be allowed to stand with a 1N HCl or HNO₃ solution for a maximum of 6 hours at room temperature, and be rinsed afterwards with purified distilled water. For trace analysis conducted in the concentration range of ng/g (ppb) or pg/g (ppt), containers made of the fluoroplastic PFA are particularly suitable, because they have a smooth surface, are easy to clean without carry-over (memory effects) and interaction with the container material.

Sterilisation of laboratory equipment made of plastics

Autoclaving

Recommended autoclaving protocol

20 minutes at 121 °C (2 bar),
according to DIN EN 285

Autoclaving (steam sterilisation) is defined as the destruction or irreversible inactivation of all reproducible microorganisms under exposure to "saturated steam at a minimum of 120 °C." (DIN 58946-1, 1987). DIN EN 285 specifies a minimum exposure time (t_g) of 20 minutes (killing time and safety margin) at a sterilisation temperature of 121 °C. For the correct sterilisation procedure, including biological safety (DIN EN 285), please contact your hygiene specialist.

Prior to autoclaving plastic labware, ensure that no soiling or residual contamination remains on the equipment. Otherwise, the residual contamination will bake on solidly during the autoclaving process. Even substances that have no effect on the plastic at room temperature can still lead to destruction of the plastic during the autoclaving process. Additionally, microorganisms might not be killed effectively if they are protected by the residual contamination.

Notes on autoclaving



- Containers with screw tops or stoppers must be **open** during autoclaving to allow for pressure equalisation
 - ➔ Autoclaving of a closed container will lead to the deformation or destruction of the container
- Plastic labware should be **stood upright on a level surface** during autoclaving to avoid shape deformation.
 - ➔ Plastic labware should not be laid on its side during autoclaving
- **No mechanical stresses** should be present during autoclaving
 - ➔ For example, do not stack items
- Do not autoclave any container that contains residual contamination or even rinsing agent
- Not all plastics are resistant to steam sterilisation! For example, polycarbonate loses its tensile strength
 - ➔ Mind the temperature limits for the plastics
 - ➔ Autoclavable products are identified with a "121 °C" symbol in this catalogue

The surfaces of some plastics can be attacked by chemicals present during autoclaving, which can cause persistent clouding. Some transparent plastics can absorb minute quantities of steam, which can lead to reversible clouding. This clouding disappears upon drying, which can be accelerated through the use of a drying oven.

Note!

For gas sterilisation, dry heat, and prior to heating in a microwave oven, all closures and stoppers must be removed as well.

Heating plastics in microwave ovens

Many plastics are suitable for use in microwave ovens. More accurate information can be obtained from the Table "Physical Properties of Plastics" on page 146. In this connection, it is important to be mindful of the chemical and temperature stability of the various plastics, and to ascertain whether the particular article and its contents are compatible with the given temperature. When aggressive acids, alkalis, or solvents are to be heated, the use of fluoroplastics is recommended. It is very important to provide for adequate ventilation (e.g., fume hoods).

Prior to the use of plastic labware in a microwave oven, the closures and stoppers must be removed from the apparatus.

Sterilisation* of plastics

Plastics	Autoclave 121 °C, t _e 20 min according to DIN	Heated air 160 °C (dry)	Gas (Ethylene oxide)	Chemical (Formalin, ethanol)	β-/γ-radiation 25 kGy
PFA	yes	yes	yes	yes	no
PTFE	yes	yes	yes	yes	no
FEP	yes	yes	yes	yes	no
ETFE	yes	no	yes	yes	no
PMP	yes	no	yes	yes	yes
PP	yes	no	yes	yes	yes (limited)
PE-HD	no	no	yes	yes	yes
PE-LD	no	no	yes	yes	yes
PC	yes ¹⁾	no	yes	yes	yes
POM	yes ¹⁾	no	yes	yes	yes (limited)
PA	no	no	yes	yes	yes
SAN	no	no	yes	yes	no
PMMA	no	no	no	yes	yes
PS	no	no	no	yes	yes
PVC	no	no	yes	yes	no
MF	no	no	yes	no	no
NR	no	no	yes	yes	no
SI	yes	-	yes	yes	no
EPDM	yes	-	yes	yes	-
FKM	yes	-	yes	yes	-

* Before sterilisation, labware must be carefully cleaned and rinsed with distilled water. Always remove covers from containers!

¹⁾ Frequent autoclaving may reduce mechanical stability!

Suitability of plastics for foodstuffs



The marked products comply with the lawful regulations of the German Consumer Goods Ordinance and/or Directives (EC) No. 1935/2004, (EC) No. 975/2009 and (EU) No. 10/2011 as amended.

In the testing for compliance with the threshold values for the global migration (or respectively, the specific migration threshold values), no determinations exceeded the allowed values. In addition, sensory testing found no olfactory and flavour-related impairments. The testing was implemented according to the 82/711/EEC and 85/572/EEC Guidelines by an independent, accredited institute.

All source materials used in the manufacturing of the products are listed in the German Consumer Goods Ordinance as at 20.12.2006, or respectively, Directive (EU) 10/2011, in accordance with the present attestation. Therefore, they represent permissible source materials in accordance with food law and may be used in the production of food commodities in accordance with the specified restrictions concerning migration threshold values and permissible residual content in the end product.

Marked PP products are suitable for contact with all foodstuff categories providing that a contact period of 24 hours and a contact temperature of 40 °C are not exceeded. Marked SAN products are suitable for contact with all aqueous, alcoholic and fatty foods, providing that a contact period of 24 hours and a contact temperature of 40 °C are not exceeded.

Disposal and Recycling of Plastics

If the disposal of a piece of plastic labware is unavoidable, regional laws and regulations must be observed. Recycling centres can be found in many cities, which are designed for the disposal of recyclable materials. To simplify the task of sorting in these recycling centres, the majority of labware from VITLAB can be easily identified and presorted by using the engraved or imprinted recycling code. Prior to disposal, plastic labware must be cleaned, and sterilised if necessary, according to the currently valid regulations.

To simplify the separation of plastics for recycling, so that these can later be reused as raw material for manufacture, plastic identification labels (number 01-07) have been introduced. This identification scheme was published in 1988 under the title "SPI resin identification coding system" by the Society of the Plastics Industry (SPI). For coding, the commonly used shorthand for plastics according to the DIN 7728 is also used.



SPI number 07 stands for "other". This is used to indicate other plastics such as PMP, PFA, PTFE etc. VITLAB doesn't use the "0"; rather, it identifies the specific raw material with the abbreviation according to DIN 7728 to simplify identification of the plastic for the end user.

CE mark / CE-IVD Guidelines

IVD Guidelines of the EU

On 7 December, 1998, the EU "Guidelines for In Vitro Diagnostic Devices" (IVD Guidelines) were published in the Official Journal of the European Communities, and thus came into force. The Guidelines were transposed into German National Law on 1 January, 2002, as a corresponding modification of the German Medical Devices Act (MPG). Consequently, in vitro diagnostic devices are considered medical devices.

Definition: Medical devices*

Medical devices are all instruments, apparatus, devices, materials, or other objects including software that are intended by the manufacturer for use in humans:

- for the purpose of detection, prevention, monitoring, treatment, alleviation or compensation of diseases, injuries or disabilities;
- for the purpose of investigation, replacement or modification of the anatomy or of a physiological process;
- for the purpose of control of conception. Pharmacologically or immunologically active agents are excluded, as these are regulated by the German Pharmaceuticals Law.

Definition: In vitro Diagnostic Devices (IVD)*

"In vitro diagnostic devices" are medical devices that are used for in vitro investigations of samples derived from the human body, including donated blood and tissue. Included are reagents, calibration substances or devices, control substances or devices, equipment, instruments, apparatus, systems, or also sample containers, if they are specifically intended by the manufacturer for use in medical tests. "In vitro diagnostic devices" serve mainly to provide information on:

- physiological or pathological conditions;
- congenital anomalies;
- monitoring of therapeutic measures.

CE Mark

With the CE mark on a product, the manufacturer affirms that the product complies with the requirements for products of that type established by the EU Guidelines and, as necessary, has undergone the required testing. The manufacturer applies this mark to the product and additionally produces a Conformity Declaration that certifies the conformity of the product with the cited guidelines and standards.

The medical products supplied by VITLAB are all included in the class of in vitro diagnostic (IVD) devices.

This includes, for example:

- VITLAB® micropipettes
- Pipette tips
- Urine bottles
- Microtubes

* See the definitions according to MPG § 3 (Definition of Terms)

Accuracy

What do “tolerance, accuracy, coefficient of variation, and precision” mean in volumetric measurements?


Graphic illustration of precision and accuracy

The dart board simulates the volume range around the centred nominal value, the white dots simulate the different measured values of a specified volume.

Good accuracy: All hits are near the centre, i.e., the nominal value.

Good precision: All hits are close together.


Result: The manufacturing process is well controlled by an accompanying quality assurance program. Minimal systematic deviations and a narrow variance in products. The permissible limits are not exceeded. There are no rejects.



Good accuracy: On average, the hits are evenly distributed around the centre.

Poor precision: No substantial errors, but hits widely scattered.


Result: All deviations are “equally probable”. Instruments exceeding the permissible tolerance should be rejected.



Poor accuracy: Although all hits are close together, the centre (nominal value) is still missed.

Good precision: All hits are close together.


Result: Improperly controlled production, with systematic deviation. Instruments exceeding the permissible tolerance should be rejected.



Poor accuracy: The hits are far removed from the centre.

Poor precision: The hits are widely scattered.

Result: These volumetric instruments are of inferior quality.



Calculation formulae

The accuracy of glass volumetric instruments is commonly defined by “Tolerance Limits”, whereas for liquid handling instruments the statistical terms “Accuracy [%]” and “Coefficient of Variation [%]” have been established.

Tolerance

The term “tolerance” (tol.) in the corresponding standards defines the maximum permissible deviation from the nominal value.

$$\text{Tol.} \geq |V_{\text{meas.}} - V_{\text{nom.}}|$$

Accuracy

Accuracy (A) indicates the closeness of measured mean volume to the nominal value, i.e., systematic measurement deviation. Accuracy is defined as the difference between the measured mean volume (\bar{V}) and the nominal value ($V_{\text{nom.}}$), related to the nominal value in percent.

$$A[\%] = \frac{\bar{V} - V_{\text{nom.}}}{V_{\text{nom.}}} \cdot 100$$

Coefficient of Variation

The coefficient of variation (CV) indicates the closeness of values from repeated measurements, i.e., random measurement deviation. The coefficient of variation is defined as standard deviation in percent, related to the mean volume.

$$CV[\%] = \frac{s \cdot 100}{\bar{V}}$$

Partial volumes

(analogous to $CV_{\text{part.}} \%$)

Generally, A and CV are based on

the nominal volume ($V_{\text{nom.}}$). These data in percent must be converted to partial volumes ($V_{\text{part.}}$). By contrast, there is no conversion for partial volumes if A and CV are stated in volume units (e.g. ml).

$$A_{\text{part.}}[\%] = \frac{V_{\text{nom.}}}{V_{\text{part.}}} \cdot A_{\text{nom.}}\%$$

Tolerance from A and CV

To a good approximation, the tolerance, e.g. for the nominal volume ($V_{\text{nom.}}$), can be calculated from the accuracy and coefficient of variation.

$$\text{Tol.} \geq \frac{|A\%| + 2CV\%}{100\%} \cdot V_{\text{nom.}}$$

Precision

If the variance in the individual measurement results about the mean volume \bar{V} is given in units of volume, this relates to precision.

Cat. No. Index

33331	24	60703	78	65975	94	73498	85	80346	97
33332	24	60795	78	65980	94	73598	85	80347	97
33333	24	60803	78	66695	81	73698	85	80348	97
36491	115	60895	78	66795	81	73898	85	80375	113
39194	60	60903	78	66895	81	75093	120	80408	109
39294	60	60995	78	66995	81	75193	120	80409	109
39394	60	61003	78	67095	81	75991	90	80410	109
39494	60	61095	78	67104	40	76299	124	80411	109
39594	60	61103	78	67195	41	77094	88	80412	109
39694	60	61195	78	67204	40	78294	89	80413	109
39794	60	61203	78	67295	41	78394	89	80418	120
39894	60	61295	78	67304	40	78593	120	80419	120
39994	60	61403	78	67395	41	78794	118	80434	119
40093	61	61495	78	67404	40	79194	52	80435	119
40193	61	61503	78	67495	41	79790	122	80436	119
40293	61	61595	78	67504	40	79890	122	80437	87
40393	61	61603	78	67595	41	79990	122	80438	87
40493	61	61695	78	67604	40	80130	99	80439	87
40593	61	61703	78	67695	41	80131	99	80440	87
40693	61	61795	78	67704	40	80134	99	80441	87
40793	61	61803	78	67795	41	80139	33	80442	87
40894	63	61895	78	67895	62	80140	33	80443	87
41094	63	64091	46	67995	62	80162	87	80445	87
41194	63	64191	46	68099	62	80164	87	80452	80
41294	63	64291	46	68199	62	80165	87	80454	80
41394	63	64391	46	68299	62	80213	124	80455	80
41494	63	64491	46	68399	62	80215	53	80456	80
41594	63	64591	46	68594	96	80217	53	80459	119
41694	63	64604	43	68894	96	80218	53	80460	119
41794	64	64614	43	69194	96	80219	53	80461	119
41894	64	64691	45	69294	96	80221	53	80462	119
41994	64	64704	43	69394	80	80222	53	80463	119
42099	64	64714	43	69493	80	80223	53	80464	119
42294	64	64791	45	70494	64	80229	94	80465	119
42393	64	64804	43	70594	64	80230	93	80466	119
42594	116	64814	43	70694	64	80231	94	80467	119
42694	116	64891	45	70794	63	80252	52	80468	119
42794	116	64904	43	70894	63	80271	91	80510	118
42894	116	64914	43	70994	63	80276	101	80511	118
42994	116	64991	45	71094	63	80277	101	80512	118
43094	116	65004	43	71194	63	80278	101	80513	118
43194	116	65014	43	71598	122	80280	116	80514	118
43610	115	65091	45	71698	122	80281	116	80515	118
44091	58	65104	43	71798	122	80282	116	80520	119
44191	58	65114	43	71898	122	80283	116	80521	119
44291	58	65191	45	71998	122	80284	116	80525	119
44391	58	65204	43	72098	122	80285	116	80526	119
44491	58	65214	43	72198	122	80286	116	80535	119
53510	75	65291	45	72298	122	80288	116	80536	119
53610	75	65304	43	72398	122	80340	97	80537	119
60503	78	65391	45	72498	122	80342	97	80550	93
60603	78	65414	43	72898	85	80343	97	80551	94
60695	78	65965	94	72998	85	80345	97	80553	94

80554	93	83313	107	95187	73	104497	98	110804	77
80555	94	83314	107	95188	71	104597	98	110904	77
80556	94	83315	107	95189	107	104997	98	110905	76
80557	94	83316	107	95193	70	105097	98	111004	77
80560	98	83317	107	95194	106	105197	98	111005	76
80562	98	90694	112	95286	75	105297	98	112197	77
80593	62	90794	112	96093	59	105597	98	112297	77
80594	62	90894	112	96293	59	105599	32	112397	77
80595	62	90994	112	96393	59	105697	98	112497	77
80596	62	91094	112	96593	59	105699	32	112597	77
80602	115	91194	112	96694	59	105799	33	112697	77
80603	115	91294	112	96794	59	105899	33	112797	77
80604	115	91394	112	97791	58	106399	32	112897	77
80730	96	91494	112	97891	58	106499	32	113197	80
80731	96	91789	109	99099	101	106599	32	113297	80
80732	96	91989	109	99199	101	106699	32	113397	80
80733	96	92089	109	99299	101	106799	32	113497	80
80734	96	92189	109	100389	110	106899	32	122097	84
80735	96	92194	112	100394	111	107097	38	122197	84
80736	96	92489	109	100489	110	107197	38	122297	84
80737	96	92689	109	100494	111	107297	38	122597	106
80828	62	92789	109	100589	13, 110	107397	38	122697	106
80877	118	92889	109	100594	111	107497	38	122797	106
80878	118	93389	107	100689	13, 110	107597	38	122897	106
80879	118	93489	107	100694	111	107797	91	130294	96
80910	95	93788	71	100789	13, 110	107897	91	130297	95
80911	95	93789	107	100889	110	107997	91	130394	96
80952	123	93793	70	100989	110	108092	105	130397	95
80953	123	93794	106	101589	110	108192	105	130494	96
80954	123	93988	71	101594	111	108292	105	130497	95
80970	89	93989	107	101689	110	108297	104	130594	96
80996	52	93993	70	101694	111	108392	105	130597	95
81056	90	93994	106	101789	13, 110	108397	104	131097	121
81213	124	94188	71	101794	111	108492	105	132193	73
81640	113	94189	107	101889	110	108497	104	132293	73
81642	113	94193	70	101894	111	108792	70	132393	73
81644	113	94194	106	101989	110	108892	70	132493	73
81646	113	94587	73	102089	13, 110	108992	70	132593	73
81660	113	94588	71	102189	13, 110	109297	104	132603	71
81662	113	94589	107	102397	105	109397	104	132605	71
81664	113	94687	73	102597	105	109497	104	132606	71
81666	113	94688	71	102697	105	109597	18, 104	132608	71
83300	72	94689	107	102897	105	109697	18, 104	132693	73
83301	72	94987	73	103297	90	109797	18, 104	132703	71
83302	72	94988	71	103397	90	110204	77	132705	71
83303	72	94989	107	103797	97	110205	76	132706	71
83304	72	94993	70	103897	97	110304	77	132708	71
83306	73	94994	106	104097	98	110305	76	132793	73
83307	73	95087	73	104099	51	110404	77	132803	71
83308	73	95088	71	104197	98	110405	76	132805	71
83310	107	95089	107	104199	51	110604	77	132806	71
83311	107	95093	70	104297	98	110605	76	132808	71
83312	107	95094	106	104397	98	110704	77	133181	69

Cat. No. Index

133281	69	155600	27	302597	82	326696	93	609941	79
133381	69	155694	27	303097	82	395940	60	610081	79
134293	72	155800	28	303197	82	395950	60	610941	79
134393	72	155894	28	303297	82	396940	60	611081	79
134493	72	155900	28	307697	83	396943	60	611941	79
134593	72	155994	28	307797	83	396944	60	612081	79
135181	69	156094	114	307897	83	396946	60	612941	79
135281	69	159497	92	307997	83	396950	60	614081	79
135381	69	159597	92	308097	83	396952	60	614941	79
136693	102	159665	88	308197	83	396955	60	615081	79
138093	108	159670	88	308297	83	397940	60	615941	79
138193	108	159697	92	308397	83	397950	60	616081	79
138293	108	160110	48	308497	83	406944	61	616941	79
138393	108	160119	48	308597	83	406950	61	617081	79
138493	108	160210	48	308897	83	407944	61	617941	79
138593	108	160219	48	308997	83	407950	61	618081	79
138693	108	160510	48	309097	83	440081	56	618941	79
138793	108	160519	48	309297	83	440941	56	640941	45
138893	108	161010	48	309397	83	441081	56	641941	45
139393	108	161019	48	310197	84	441941	56	642941	45
139493	108	162510	48	310297	84	442081	56	643941	45
139593	108	163094	47	310397	84	442941	56	644941	45
139693	108	163194	47	310497	84	443081	56	645941	45
139793	108	163294	47	311097	82	443941	56	646081	44
139893	108	163394	47	311197	82	444081	56	646941	44
145094	100	163594	47	311297	82	444941	56	647081	44
145194	100	164094	47	311397	82	445081	56	647941	44
146294	28	164194	47	311497	82	445941	56	648081	44
146494	28	164294	47	311597	82	446081	56	648941	44
148893	74	164394	47	311697	82	446941	56	649081	44
148894	27	164494	47	311797	82	447081	56	649941	44
148993	74	164594	47	316097	83	447941	56	650081	44
148994	27	165094	116	316197	83	480941	57	650941	44
149093	74	165194	116	316297	83	481941	57	651081	44
149094	28	165294	116	316397	83	481942	57	651941	44
149193	74	165394	116	316497	83	481943	57	652081	44
149194	28	165494	116	318293	85	481944	57	652941	44
149293	74	165594	116	318393	85	481945	57	653081	44
149393	74	300497	82	318597	84	482941	57	653941	44
149693	74	300597	82	319099	25	482942	57	666941	81
149794	27	300897	82	324594	51	482943	57	667941	81
149893	74	301097	82	324694	51	482944	57	668941	81
149993	74	301197	82	324794	51	482945	57	669941	81
149994	27	301597	82	325095	87	483941	57	670040	39
150094	28	301697	82	325195	87	484941	57	670941	81
150194	28	301797	82	325295	87	605081	79	670950	39
150294	28	301897	82	325395	87	606081	79	671040	39
150394	28	301997	82	325495	87	606941	79	671891	42
151594	114	302097	82	326094	93	607081	79	671895	41
155094	114	302197	82	326194	93	607941	79	671941	42
155400	27	302297	82	326294	93	608081	79	671950	39
155494	27	302397	82	326496	93	608941	79	672040	39
155594	114	302497	82	326596	93	609081	79	672891	42

<u>672895</u>	<u>41</u>	<u>1332899</u>	<u>67</u>	<u>1602504</u>	<u>12</u>	<u>1650110</u>	<u>15</u>	<u>1672015</u>	<u>25</u>
<u>672941</u>	<u>42</u>	<u>1332909</u>	<u>67</u>	<u>1602505</u>	<u>12</u>	<u>1650111</u>	<u>14</u>	<u>1672016</u>	<u>25</u>
<u>672950</u>	<u>39</u>	<u>1332939</u>	<u>67</u>	<u>1605503</u>	<u>12</u>	<u>1655075</u>	<u>16</u>	<u>3125970</u>	<u>84</u>
<u>673040</u>	<u>39</u>	<u>1332949</u>	<u>67</u>	<u>1605504</u>	<u>12</u>	<u>1655080</u>	<u>16</u>	<u>3126970</u>	<u>84</u>
<u>673891</u>	<u>42</u>	<u>1332959</u>	<u>67</u>	<u>1605505</u>	<u>12</u>	<u>1655095</u>	<u>16</u>	<u>3190940</u>	<u>99</u>
<u>673895</u>	<u>41</u>	<u>1332969</u>	<u>67</u>	<u>1605506</u>	<u>12</u>	<u>1655100</u>	<u>16</u>	<u>3190941</u>	<u>100</u>
<u>673941</u>	<u>42</u>	<u>1332979</u>	<u>67</u>	<u>1605507</u>	<u>12</u>	<u>1670050</u>	<u>25</u>	<u>3190943</u>	<u>99</u>
<u>673950</u>	<u>39</u>	<u>1333819</u>	<u>67</u>	<u>1605508</u>	<u>12</u>	<u>1670066</u>	<u>14, 31</u>	<u>3190948</u>	<u>99</u>
<u>674040</u>	<u>39</u>	<u>1333839</u>	<u>67</u>	<u>1607515</u>	<u>17</u>	<u>1670067</u>	<u>14, 31</u>	<u>3191940</u>	<u>99</u>
<u>674891</u>	<u>42</u>	<u>1333849</u>	<u>67</u>	<u>1607525</u>	<u>17</u>	<u>1670068</u>	<u>14, 31</u>	<u>3191943</u>	<u>99</u>
<u>674895</u>	<u>41</u>	<u>1333859</u>	<u>67</u>	<u>1607535</u>	<u>17</u>	<u>1670072</u>	<u>19</u>	<u>3191948</u>	<u>99</u>
<u>674941</u>	<u>42</u>	<u>1333869</u>	<u>67</u>	<u>1607545</u>	<u>17</u>	<u>1670080</u>	<u>19, 31</u>	<u>3192940</u>	<u>99</u>
<u>674950</u>	<u>39</u>	<u>1351819</u>	<u>68</u>	<u>1608000</u>	<u>23</u>	<u>1670085</u>	<u>31</u>	<u>3192943</u>	<u>99</u>
<u>675040</u>	<u>39</u>	<u>1351839</u>	<u>68</u>	<u>1608002</u>	<u>23</u>	<u>1670090</u>	<u>19, 31</u>	<u>3192948</u>	<u>99</u>
<u>675891</u>	<u>42</u>	<u>1351849</u>	<u>68</u>	<u>1608004</u>	<u>23</u>	<u>1670092</u>	<u>19</u>	<u>3193940</u>	<u>99</u>
<u>675895</u>	<u>41</u>	<u>1351859</u>	<u>68</u>	<u>1608006</u>	<u>23</u>	<u>1670095</u>	<u>31</u>	<u>3193943</u>	<u>99</u>
<u>675941</u>	<u>42</u>	<u>1351869</u>	<u>68</u>	<u>1608008</u>	<u>23</u>	<u>1670100</u>	<u>19, 31</u>	<u>3193948</u>	<u>99</u>
<u>675950</u>	<u>39</u>	<u>1352819</u>	<u>68</u>	<u>1610501</u>	<u>20</u>	<u>1670105</u>	<u>19</u>	<u>3194940</u>	<u>99</u>
<u>676040</u>	<u>39</u>	<u>1352839</u>	<u>68</u>	<u>1610502</u>	<u>20</u>	<u>1670110</u>	<u>14, 31</u>	<u>3194943</u>	<u>99</u>
<u>676891</u>	<u>42</u>	<u>1352849</u>	<u>68</u>	<u>1610503</u>	<u>20</u>	<u>1670115</u>	<u>19, 31</u>	<u>3194948</u>	<u>99</u>
<u>676895</u>	<u>41</u>	<u>1352859</u>	<u>68</u>	<u>1610504</u>	<u>20</u>	<u>1670120</u>	<u>14, 31</u>	<u>3195940</u>	<u>99</u>
<u>676941</u>	<u>42</u>	<u>1352869</u>	<u>68</u>	<u>1610506</u>	<u>20</u>	<u>1670125</u>	<u>19, 31</u>	<u>3195943</u>	<u>99</u>
<u>676950</u>	<u>39</u>	<u>1352879</u>	<u>68</u>	<u>1611503</u>	<u>20</u>	<u>1670145</u>	<u>20</u>	<u>3195948</u>	<u>99</u>
<u>677891</u>	<u>42</u>	<u>1352889</u>	<u>68</u>	<u>1611506</u>	<u>20</u>	<u>1670150</u>	<u>14</u>	<u>3197940</u>	<u>100</u>
<u>677895</u>	<u>41</u>	<u>1352899</u>	<u>68</u>	<u>1611508</u>	<u>20</u>	<u>1670155</u>	<u>14, 31</u>	<u>3197943</u>	<u>100</u>
<u>677941</u>	<u>42</u>	<u>1352909</u>	<u>68</u>	<u>1612000</u>	<u>23</u>	<u>1670165</u>	<u>14</u>	<u>3197948</u>	<u>100</u>
<u>760941</u>	<u>46</u>	<u>1352939</u>	<u>68</u>	<u>1612002</u>	<u>23</u>	<u>1670170</u>	<u>14</u>	<u>3198940</u>	<u>100</u>
<u>833019</u>	<u>69</u>	<u>1352949</u>	<u>68</u>	<u>1612004</u>	<u>23</u>	<u>1670175</u>	<u>14</u>	<u>3198943</u>	<u>100</u>
<u>833029</u>	<u>69</u>	<u>1352959</u>	<u>68</u>	<u>1612006</u>	<u>23</u>	<u>1670180</u>	<u>14, 31</u>	<u>3198948</u>	<u>100</u>
<u>833039</u>	<u>69</u>	<u>1352969</u>	<u>68</u>	<u>1612008</u>	<u>23</u>	<u>1670647</u>	<u>50</u>	<u>3961111</u>	<u>60</u>
<u>833049</u>	<u>69</u>	<u>1352979</u>	<u>68</u>	<u>1620506</u>	<u>30</u>	<u>1670648</u>	<u>50</u>	<u>4811111</u>	<u>57</u>
<u>952861</u>	<u>75</u>	<u>1353819</u>	<u>68</u>	<u>1620507</u>	<u>30</u>	<u>1670650</u>	<u>50</u>	<u>4821111</u>	<u>57</u>
<u>978081</u>	<u>58</u>	<u>1353839</u>	<u>68</u>	<u>1630500</u>	<u>50</u>	<u>1670660</u>	<u>50</u>		
<u>978941</u>	<u>58</u>	<u>1353849</u>	<u>68</u>	<u>1631500</u>	<u>49</u>	<u>1670700</u>	<u>18</u>		
<u>1017940</u>	<u>111</u>	<u>1353859</u>	<u>68</u>	<u>1631510</u>	<u>49</u>	<u>1671050</u>	<u>18</u>		
<u>1018940</u>	<u>111</u>	<u>1353869</u>	<u>68</u>	<u>1631520</u>	<u>49</u>	<u>1671055</u>	<u>18</u>		
<u>1019940</u>	<u>111</u>	<u>1431829</u>	<u>67</u>	<u>1631530</u>	<u>49</u>	<u>1671080</u>	<u>19</u>		
<u>1037979</u>	<u>97</u>	<u>1432829</u>	<u>67</u>	<u>1631540</u>	<u>49</u>	<u>1671082</u>	<u>19</u>		
<u>1038971</u>	<u>97</u>	<u>1432989</u>	<u>67</u>	<u>1641000</u>	<u>22</u>	<u>1671083</u>	<u>19</u>		
<u>1327111</u>	<u>71</u>	<u>1433829</u>	<u>67</u>	<u>1641002</u>	<u>22</u>	<u>1671085</u>	<u>15, 31</u>		
<u>1328111</u>	<u>71</u>	<u>1433959</u>	<u>67</u>	<u>1641004</u>	<u>22</u>	<u>1671086</u>	<u>19</u>		
<u>1331819</u>	<u>67</u>	<u>1451829</u>	<u>68</u>	<u>1641006</u>	<u>22</u>	<u>1671095</u>	<u>14, 31</u>		
<u>1331839</u>	<u>67</u>	<u>1452829</u>	<u>68</u>	<u>1641008</u>	<u>22</u>	<u>1671116</u>	<u>13, 18</u>		
<u>1331849</u>	<u>67</u>	<u>1452989</u>	<u>68</u>	<u>1641010</u>	<u>22</u>	<u>1671500</u>	<u>13, 31</u>		
<u>1331859</u>	<u>67</u>	<u>1453829</u>	<u>68</u>	<u>1641012</u>	<u>22</u>	<u>1671505</u>	<u>13</u>		
<u>1331869</u>	<u>67</u>	<u>1453959</u>	<u>68</u>	<u>1650020</u>	<u>15</u>	<u>1671506</u>	<u>13</u>		
<u>1332819</u>	<u>67</u>	<u>1601503</u>	<u>12</u>	<u>1650025</u>	<u>15</u>	<u>1671510</u>	<u>13, 31</u>		
<u>1332839</u>	<u>67</u>	<u>1601504</u>	<u>12</u>	<u>1650030</u>	<u>15</u>	<u>1671515</u>	<u>13</u>		
<u>1332849</u>	<u>67</u>	<u>1601505</u>	<u>12</u>	<u>1650035</u>	<u>15</u>	<u>1671520</u>	<u>13</u>		
<u>1332859</u>	<u>67</u>	<u>1601506</u>	<u>12</u>	<u>1650080</u>	<u>15</u>	<u>1672000</u>	<u>25</u>		
<u>1332869</u>	<u>67</u>	<u>1601507</u>	<u>12</u>	<u>1650085</u>	<u>15</u>	<u>1672002</u>	<u>25</u>		
<u>1332879</u>	<u>67</u>	<u>1601508</u>	<u>12</u>	<u>1650086</u>	<u>14</u>	<u>1672010</u>	<u>25</u>		
<u>1332889</u>	<u>67</u>	<u>1602502</u>	<u>12</u>	<u>1650100</u>	<u>15</u>	<u>1672012</u>	<u>25</u>		

Alpha - Index

2-way connector, PE-HD 119

A

Accessories for VITLAB[®] pipeo[®] & maneus[®] 50
Accessories for VITLAB[®] microlitre pipettes 25
Adapter for VITLAB[®] continuous E/RS 31
Adapter for VITLAB[®] genius and simplex 14
Adapter for VITLAB[®] piccolo 20
Adapter for VITLAB[®] TA 19
Analytical funnels, PP 87
Autosampler-vials, PFA 98

B

Beakers 56 - 58, 76 - 80
Bottle-top burette VITLAB[®] continuous 30
Bottle-top dispenser VITLAB[®] genius 12
Bottle-top dispenser VITLAB[®] piccolo 20
Bottle-top dispenser VITLAB[®] simplex 12
Bottle-top dispenser VITLAB[®] TA 17
Bottles 66 - 73, 104 - 113
Bottles for VITLAB[®] continuous E/RS 31
Bottles for VITLAB[®] genius and simplex 13
Bowl, PP, with lid 115
Bowls, PP 116
Büchner funnels, PP 87
Bucket with spout, PP 59
Buckets, PE-HD 59
Bulb pipettes, PP, Class B 47
Burette clamps, PP 33
Burette stopcocks, PMP/PTFE 33
Burette VITLAB[®] continuous 30
Burettes, borosilicate glass 3.3 32
Burettes, VITLAB[®] Dr. Schilling 32

C

Cans 95 - 98
Caps with dropper inserts, PE-HD 73
Catchment trays, PP 116
Chemical waste disposal system, PE/PP 114
Collectors, PP or SAN 58
Coloured wash-bottles, PE-LD/PP 71
Connectors 118, 119
Connectors, straight, PP 118
Connectors, T-shape, PP 119
Connectors, universal PP 118
Connectors, Y-shape, PP 119
Container, PP 114
Coplín staining chamber, PP 102

D

Desiccator plates, PP and porcelain 94
Desiccators with stopcock, PC 93
Desiccators with stopcock, PP/PC 93
Desiccators, PP/PC 93
Discharge tube for VITLAB[®] genius and simplex 14, 15
Discharge valves for VITLAB[®] genius and simplex 16
Dishes 80, 116, 122
Dishes, PVC 116
Dispenser VITLAB[®] genius 12
Dispenser VITLAB[®] piccolo 20
Dispenser VITLAB[®] simplex 12
Dispenser VITLAB[®] TA 17
Dispensing cartridge for VITLAB[®] TA 18
Disposable pipettes, PS 48
Double spatula 62
Drawer organisers, PVC 123
Dropping bottles, PE-LD 73
Dropping bottles, PE-LD/PE-HD 73
Dropping pipettes 74
Drying racks 124
Drying tube for VITLAB[®] continuous E/RS 31
Drying tube for VITLAB[®] genius and simplex 14

E

Erlenmeyer flasks 81
Evaporating dishes, PFA 90

F

Filling tubes for VITLAB[®] genius and simplex 15
Filtering rack 89
Forceps 62
Funnels 63, 64, 87
Funnels, PP 63

G

Gas wash bottles, PFA 92
Graduated beakers, coloured, PP 57
Graduated beakers, PP 56, 57
Graduated beakers, SAN 58
Graduated beakers, stackable, PP 57
Graduated cylinders, PMP, Class A, tall shape 43
Graduated cylinders, PP, Class B, short shape 45
Graduated cylinders, PP, Class B, tall shape 44
Graduated cylinders, SAN, Class B, short shape 46
Graduated cylinders, SAN, Class B, tall shape 45
Graduated pipettes 47, 48
Graduated pipettes, PP, Class B 47
Griffin beakers, ETFE 77
Griffin beakers, PFA 76
Griffin beakers, PMP 78
Griffin beakers, PP 79
Griffin beakers, PTFE 77

H

Hydrometer cylinder, PP 46

I

Imhoff cone, SAN 90

L

Laboratory trays, PP 116
Large funnels, PE-HD 64
Large funnels, PP 64
Lids for trays, PS 122

M

Magnetic stir bar, triangular, PTFE 84
Magnetic stir bars 82 - 84
Magnetic stirring bar retrievers, flexible, PTFE 84
Magnetic stirring bar retrievers, PE 85
Magnetic stirring bar retrievers, PTFE 84
Magnetic stirring bars, barbell, PTFE 84
Magnetic stirring bars, cross shape, PTFE 83
Magnetic stirring bars, octagonal, PTFE 83
Magnetic stirring bars, oval, PTFE 82
Magnetic stirring bars, polygonal, PTFE 82
maneus[®] 50
Measuring cup, PP 80
Measuring scoops, coloured, PP 60
Measuring scoops, PP 60
Microlitre pipettes 22, 23
Microtube stands 100
Microtubes, PP 100
Mortars, MF 85
Multi-channel pipettes 23
Multi-purpose container, SAN 115

N

Narrow-mouth bottles 104 - 109
Narrow-mouth bottles, PE-HD 109
Narrow-mouth bottles, PE-LD 107, 108
Narrow-mouth bottles, PFA 104
Narrow-mouth bottles, PP 106
Non-return valves 120

O

O-rings for desiccators 94

P

Pasteur pipettes 74
 Pestles, MF 85
 PFA-economy narrow-mouth bottles 105
 PFA-economy wash bottles 70
 pipeo® 49
 Pipette baskets 53
 Pipette fillers 51
 Pipette jars 53
 Pipette stands 52
 Pipette tips, PP 26 - 28
 Pipette trays 52
 Pipette washer 53
 Pipettes 47, 48, 74
 Pipettes, Piston-operated pipettes 22, 23
 Piston-operated pipettes 22, 23
 Plastic stand for VITLAB® dispensers 13
 Plastic stand for VITLAB® TA 18
 Powder funnels, PP 63
 PTFE-tape 121

R

Reagent bottles, opaque, PP, wide mouth 111
 Reagent bottles, PP 110, 111
 Reagent reservoir 25
 Reagent tube racks 98, 99
 Recirculation valve for VITLAB® TA 18
 Round-bottom flask stand 91
 Round-bottom flasks, PFA 91

S

Safety wash bottles, VITsafe™ 66 - 72
 Sample containers 95 - 98
 Sample containers, PE-HD 95
 Sample containers, PE-LD 96
 Sample containers, PFA 95
 Sample containers, PP 96
 Sample tubes, PFA 97
 Sample vials, PFA 98
 Scoops 60, 61
 Scoops, PE-HD 61
 Screw caps, PFA 105
 Screw caps, PP 107
 Sealing tape, PTFE 121
 Sedimentation cone, SAN 90
 Sedimentation rack 90
 Slide storage boxes, PS 101
 Spatula 62
 Spatula spoon 62
 Spray bottles 75
 Spray bottles, PP 75
 Staining chamber for slides, POM 101
 Staining jar for slides, POM 101
 Staining rack for slides, POM 101
 Standard joint funnels, PP 64
 Standard joint stoppers, PP 112
 Starter-Sets VITLAB® micropipette 24
 Stir bars, magnetic 82 - 84
 Stirring rod, PP 62
 Stopper, PP, Standard joint 112
 Storage bottles, PE-HD, with tap 113
 Storage bottles, PE-HD, without tap 113
 Support for separatory funnels 89

T

Tap for storage bottles, PP 113
 Telescopic filling tube for VITLAB® continuous E/RS 31
 Telescoping filling tube for VITLAB® TA 19
 Test tube racks, coloured, PP 99
 Threaded bottles for VITLAB® continuous E/RS 31
 Tip-Box 5/10 ml 26
 Tip-Box N 26
 Transport container, PE-HD 115
 Trays, MF 122
 Tubing connectors 118, 119

U

Urbanti funnels, PMP 87

V

Valve for desiccators 94
 VENT-CAP wash bottle caps 69
 VITLAB maneus® 50
 VITLAB maneus® pipette helper 50
 VITLAB pipeo® 49
 VITLAB pipeo® pipette helper 49
 VITLAB® continuous E/RS 30
 VITLAB® Dr. Schilling burettes 32
 VITLAB® genius 12
 VITLAB® micropipette -8/-12 23
 VITLAB® micropipette Starter-Sets 24
 VITLAB® micropipettes 22
 VITLAB® opaque volumetric flasks, PMP, Class A 39
 VITLAB® piccolo 20
 VITLAB® simplex 12
 VITLAB® TA 17
 VITsafe™ safety wash bottles, narrow-mouth 67
 VITsafe™ safety wash bottles, wide-mouth 68
 Volumetric flasks, PFA, Class A 38
 Volumetric flasks, PMP, Class A 40
 Volumetric flasks, PMP, Class B 41
 Volumetric flasks, PP, Class B 42

W

Wash bottle caps, PP 72
 Wash bottle caps, VENT-CAP 69
 Wash bottles with imprint, PE-LD/PP 69
 Wash-bottles 66 - 72
 Wash-bottles, PE-LD 72
 Wash-bottles, PE-LD/PP 71
 Wash-bottles, PP 70
 Wash-bottles, VITsafe™ 66 - 72
 Watch glasses, PP 80
 Watch glasses, PTFE 80
 Water flow stopcocks, PE 120
 Water-jet pump, PP 88
 Weighing jars, PP 97
 Wide-mouth bottles 18, 104, 106 - 109
 Wide-mouth bottles, PE-HD 109
 Wide-mouth bottles, PE-LD 107 - 109
 Wide-mouth bottles, PE-LD, with eye closure 109
 Wide-mouth bottles, PFA 18, 104
 Wide-mouth bottles, PP 106
 Wide-mouth bottles, PTFE 106

General Terms and Conditions of VITLAB GmbH

1. General

- 1.1 These General Terms and Conditions (GT&C) are intended for use in commercial transactions between businesses.
- 1.2 These GT&C shall apply for all, including future, contracts with the customer. Other terms and conditions shall not become part of the contract, even if we do not expressly object to them. Subsidiary agreements made before or at the time of conclusion of contract may only be invoked if they are immediately confirmed in writing. The waiver of the requirement for written form shall only be possible in writing. The language of the contract shall be German or English. In the event of a discrepancy between the German language version of these GT&C and a version in any language, the German language version shall prevail.
- 1.3 Our offers are subject to change and non-binding. We reserve the right to make technical improvements to our products.
- 1.4 We may store and process data in our IT system necessary for the purpose of processing the contract.
- 1.5 A set-off by the customer shall not be permitted unless the counterclaims are undisputed or legally established, or pecuniary counterclaims arising from the right to refuse payment pursuant to Section 320 Bürgerliches Gesetzbuch (BGB) (German Civil Code).
- 1.6 Orders with a goods value of below € 250 shall be subject to a minimum order surcharge of € 50. Delivery shall be undertaken generally in packaging units (PU) according to the currently valid price list. For deliveries within five (5) working days or for order values up to € 500, we reserve the right to waive an order confirmation.
- 1.7 The place of jurisdiction shall be the court responsible for our head office in Aschaffenburg, Germany. We shall also be entitled to appeal to the court responsible for the head office of our customer. We shall, furthermore, as plaintiffs have the right to invoke the Arbitration Court at the Chamber of Commerce and Industry in Frankfurt am Main, Germany. The Arbitration Court shall, in this case, make the final judgment in accordance with the Rules of Arbitration of the Chamber of Commerce and Industry in Frankfurt am Main without recourse to the ordinary courts of law. The instigation of legal dunning proceedings by us shall not signify the exertion of our right of choice; it shall be admissible in all cases.
- 1.8 German law shall apply exclusively under the exclusion of the conflict of laws principles of Private International Law and the UN Convention on Contracts for International the Sale of Goods (CISG).

2. Delivery

- 2.1 The place of performance shall be our factory in Grossostheim, Germany. The risk shall transfer to the customer when the delivery leaves the ramp at our factory. This shall also apply to partial deliveries or where we have performed additional services, such as shipping; costs for transport, packaging or insurance; exportation and installation.
- 2.2 Insofar as we have agreed to orders on call, the customer must take delivery of the total amount within six (6) months, at the latest at the date confirmed by us.
- 2.3 In the case of a delay in the customer's acceptance of a delivery, we may, without prejudicing our claim for performance, have the goods put into storage at the cost of the customer or, after providing a warning and setting a deadline for the customer, otherwise dispose of them.

3. Delivery Period, Delay

- 3.1 Delivery times shall be ex works. Delivery periods shall begin on receipt of our order confirmation by the customer; however only after settlement of any technical issues pending from the conclusion of the contract; and after receipt of any documents to be provided to us by the customer, such as drawings, permits or approvals; and definitely not before receipt of agreed advance payments. The delivery period shall be considered to have been met if readiness for dispatch has been notified before the expiry of this period. Delivery shall be subject to us receiving our own supplies punctually and in good order.
- 3.2 Force Majeure and circumstances beyond our control, such as strikes, lock-outs, operational disruption, shortages of raw materials and equipment, delayed delivery or non-delivery by our suppliers, shall extend the delivery periods accordingly and shall release us from our delivery obligations if they, as a result, render delivery impossible. We shall also not be liable for the circumstances described above if they arise during an already existing delay. The same shall apply for any additional or amended services requested by the customer.
- 3.3 We shall be considered to be in default of delivery only if the customer has issued us with a reminder, has set a reasonable extension period which has elapsed.
- 3.4 In the case of delay damages, our liability for compensation shall be limited to 10% of the value of the delayed delivery/service. The limitation shall not apply in cases of wilful intent, gross negligence and/or injury to life, limb or health. The customer shall be obliged to immediately inform us in writing of any likely consequences of delay.

4. Prices, Terms of Payment

- 4.1 Prices shall be ex works and exclusive of statutory VAT, if applicable. Costs of packaging, transportation, freight and insurance shall be borne by the customer. Prices shall also be exclusive of the cost of returning and recycling/dumping of old equipment.
- 4.2 Invoices shall be payable to our account in EUROs (€) without deductions and free of charges and expenses. Payment shall be made immediately or by the date stated. The determinant factor shall be the receipt of payment. Cheques and bills of exchange shall only be accepted on account of performance and at the cost of the customer.
- 4.3 In the case of customers, with whom we are working for the first time or with whom we do not work regularly, after delay in payment or in the case of reasonable doubt as to the creditworthiness of the customer, we shall reserve the right to make individual deliveries dependent on their pre-payment or a security deposit to the value of the invoice amount.
- 4.4 Should the period between conclusion of contract and agreed delivery exceed four (4) months, so may we, at our discretion, demand a reasonable additional charge equivalent to the increase in our costs up until delivery. For deliveries on call, our current price shall apply.
- 4.5 In the case of an agreed return of goods that are free of defects, the customer shall be charged a checking and processing fee of 20 % of the invoice amount (minimum € 50).
- 4.6 Should the customer be in arrears with payment, our debt claims against him shall be due immediately, and we shall not be obliged to make any further deliveries based on current delivery contracts.
- 4.7 If payment is delayed, we shall charge - notwithstanding further damage compensation claims - interest on arrears at the statutory rate.
- 4.8 We may offset amounts payable to the customer (e.g. from credit notes) against our claims against the customer.

5. Retention of Title, Assignment of Future Claims

- 5.1 The goods delivered shall remain our property until the complete and unlimited payment. Should we still have further claims against the customer, we shall then retain our property rights until payment of these has been effected.
- 5.2 The customer may neither use goods subject to retention of title nor combine them with other objects to which a third party may have rights. Should, however, goods subject to retention of title become, through their combination with other objects, part of a new (complete) item, we shall be a proportional co-owner of this new item directly, even if this latter component is regarded as the main component. Our proportion of co-ownership shall be determined by the ratio of the invoice value of the goods to the value of the new item at the time of combination.
- 5.3 The customer may resell goods subject to retention of title in the course of his normal business as long as he has not assigned, pledged or otherwise encumbered his claims from the resale.
- 5.4 The customer shall assign to us in advance as collateral any claims against his customers from the resale of the goods subject to retention of title (see Clause 5.3) and/or newly formed items (see Clause 5.2) to the value of our invoice for the goods subject to retention of title. As long as the customer is not in default of payment for the goods subject to retention of title, he may collect the assigned claims in the ordinary course of business. He may, however, only use the proportional proceeds for the payment to us for the goods subject to retention of title.
- 5.5 At the customer's request, we shall release collateral at our discretion if and to the extent that the nominal value of the collateral exceeds 120% of the nominal value of our outstanding debt claims against the customer.
- 5.6 The customer shall be required to inform us immediately of any attachments, seizures or any other third-party dispositions relating to the goods that are reserved or co-owned by us.

- 5.7 In the event of failure to pay bills of exchange or cheques, or failure or recall of a payment made by debit order/direct debit mandate, suspension of payments or insolvency of the customer or of the end buyer, the rights of the customer under Clause 5.3 shall no longer be valid. The customer must then immediately inform the buyer of our extended retention of title; he may use the assignment of relevant proportional proceeds only to pay for the delivered goods.
- 5.8 Where payment is delayed and in the cases covered in Clause 5.7, we shall be entitled to withdraw from the contract and/or, without withdrawing from the contract, demand the return of any goods subject to retention of title still in possession of the customer and to collect the assigned receivables ourselves. In order to ascertain our rights, we shall be entitled to have all of our customer's documents/books concerning our reserved rights examined by a person who is subject to the professional duty of confidentiality.

6. Warranty, Limitation of Liability

- 6.1 We warrant that our delivered goods (including any agreed installation) are free of defects at time of risk transfer. The required quality, durability and use of our delivered goods are based solely on the agreed written specification, product description and/or operating manuals. Any information beyond this, in particular in preliminary discussions, advertising and/or referencing industrial standards shall only become part of the contract if they are expressly referenced in writing.
- 6.2 Should the customer requires the delivered goods for purposes other than those agreed, he must take responsibility himself for examining their special suitability for this - also in terms of product safety - and ensure their compliance with all relevant technical, legal or regulatory provisions before the intended use. We shall not be liable for any usability that was not expressly confirmed by us in writing. In the case of material or design requirements of the customer, we shall accept no liability for the suitability or permissibility of the desired materials or designs, and shall, in this respect, have no particular testing obligation. Compliance with safety-related and occupational health regulations depends on the location and operating conditions of which we have no prior knowledge. Action for ensuring compliance shall therefore be the responsibility of the customer or his buyer.
- 6.3 We shall not be liable for the consequences of improper handling, use, maintenance and operation of the delivered goods; the consequences of normal wear and tear, in particular of wearing parts, such as pistons, seals, valves; the breakage of glass, plastic or ceramic parts; for the consequences of chemical, electrochemical or electrical influences; or non-observance of the operating instructions.
- 6.4 If a notice of defect is justified, we shall initially only be required to provide supplementary performance. Supplementary performance shall be, at our discretion, either rectification of the defect or delivery of goods free of defects. Further warranty claims shall only apply in the event of rejection, impossibility or failure of the supplementary performance. The customer shall bear additional expenses, which arise from the fact that the goods were taken after delivery to a location other than the agreed place of performance.
- 6.5 The customer must, immediately upon receipt of the goods, inspect them carefully, also in terms of product safety, and notify obvious defects immediately in writing; any hidden defects must be immediately notified upon discovery. The customer must notify the carrier immediately of any transport damage. Failure to observe the testing and notification obligation shall void any customer claims for defects.
- 6.6 Our liability for slight negligence shall be limited to claims for injury to life, limb or health, to claims under the Produkthaftungsgesetz (German Product Liability Act) or to claims of culpable breach of fundamental contractual obligations through which the purpose of the contract is endangered. Otherwise, our liability for slightly negligent breach of fundamental contractual obligations is limited to the typically occurring damages which we could have foreseen when the contract was concluded.
- 6.7 Should the customer use the delivered goods in conjunction with environmentally harmful, toxic, radioactive or otherwise hazardous materials, he shall be obliged to clean them before returning them to us. If applicable, we may charge any necessary costs for decontamination/cleaning and disposal to the customer's account.

7. Limitation Period

The warranty period shall be one year and starts from the date of delivery of the goods to the customer. The same shall apply for claims for damages, irrespective of their legal basis. The limitation periods of Section 438 Para. 1 Nos. 1 and 2, Section 479 Para. 1 and Section 634a Para. 1 No. 2 of the BGB (German Civil Code) shall remain unaffected. The restriction of the limitation period shall not apply to claims based on fraudulent concealment of a defect, for claims under the Produkthaftungsgesetz (German Product Liability Act) or for damages resulting from injury to life, limb or health and other damages based on intent or gross negligence. The limitation period in respect of replaced or repaired goods shall not commence anew.

8. Software Use

- 8.1 If software is included in the scope of a delivery, the customer shall be granted a non-exclusive right to use the software and its associated documentation. It is provided for use on the designated delivery item. The use of the software on more than one system shall be prohibited.
- 8.2 The customer shall only be entitled to copy, transfer or translate the software or to convert it from object code to source code to the extent permitted by law (Sections 69a et seq. Urheberrechtsgesetz - German Copyright Act). The customer undertakes to refrain from removing manufacturer information, in particular copyright notices, or from changing these without our prior express consent or the prior express consent of the software supplier.
- 8.3 All other rights to the software and the documentation including copies thereof shall remain with us and/or the software supplier. The issue of sub-licences is not permitted.

9. Installation

- 9.1 Installation costs may be invoiced on a monthly basis. Fixed installation prices shall only cover the work that has been agreed upon. In other cases our current price list for installation and service costs shall apply.
- 9.2 The customer shall be responsible for providing the following at his own expense: lighting, motive power, if necessary, compressed air, water, electrical power for welding and heating, including the necessary connections; electrical installations to connect the products supplied by us; the devices required (such as lifting equipment); a lockable room that can be used for storing materials; tools and clothing during the installation.

10. Spare Parts, Maintenance/Repair and Calibration

- 10.1 For spare parts and maintenance, repair and calibration services, the current repair and exchange price list shall apply.
- 10.2 Insofar as there is an obligation on our part to maintain/supply spare parts, then this obligation shall be limited to a period of five (5) years from the date of delivery. If spare parts are not manufactured by us, or are no longer available on the market, for example electronic components, or if the raw material for their production is no longer available, our obligation to deliver spare parts shall lapse.
- 10.3 For calibration and maintenance, expendable items from VITLAB production are normally used.
- 10.4 Maintenance and calibration services can only be provided if the customer has declared the devices sent to be safe to work on from a health hazard perspective.
- 10.5 For repair/service values of up to € 50, we reserve the right not to provide a separate cost estimate.

11. Legal Reservation, Industrial Property Rights, Confidentiality

- 11.1 We reserve ownership and all industrial property rights and copyrights to all moulds, tools or other devices, samples, pictures, and business and technical documents produced or provided by us. This also applies where the customer has wholly or in part taken on the costs hereof. The customer may use these only in the manner agreed with us. Without our written consent, he may not himself manufacture contractual objects delivered or have the same manufactured by third parties.
- 11.2 Insofar as we deliver goods according to the designs or other requirements specified by the customer (models, patterns etc.), the customer shall be liable to us by default for ensuring that, through the manufacture and delivery of these goods, the industrial property rights or other rights of third parties are not infringed. If the customer is at fault he shall reimburse us all damage resulting from any such infringement of rights.
- 11.3 Any information acquired from this business relationship and not deemed to be public knowledge must not be disclosed by the customer to third parties.

Status as of: January 2014

VITLAB GmbH

Linus-Pauling-Str. 1
63762 Grossostheim

Germany

tel: +49 (0) 6026 9 77 99-0

fax: +49 (0) 6026 9 77 99-30

e-mail: info@vitlab.com

www.vitlab.com

USt.-IdNr. / VAT REG NO

DE 1116669 59

WEEE-Reg.-Nr. DE 30031601

Banking details

Sparkasse Aschaffenburg

Deutsche Postbank AG

Commerzbank AG

Deutsche Bank AG

IBAN

DE91 7955 0000 0000 0003 15

DE71 5001 0060 0040 0016 06

DE63 7908 0052 0309 9404 00

DE49 5087 0005 0010 5619 00

SWIFT-BIC

BYLA DE M1 ASA

PBNK DE FF

DRES DE FF 790

DEUT DE FF 508